



File ..\DATA\2020\20200526\974\BIZ2020-525-SCH2-.D Tgt Mass (CHM):  
 Injection Date : 26 May 20 11:19 pm +0800 Seq. Line : 158  
 Sample Name : BIZ2020-525-SCH2 Location : P1-D-06  
 Acq. Operator : ZJ\_1432 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 0.5 ul  
 Acq. Method : D:\Chem32\1\data\2020\20200526\974\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2020\20200526\974\1-POS-3MIN.M  
 Catalog No : HY-19123  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-607  
 Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

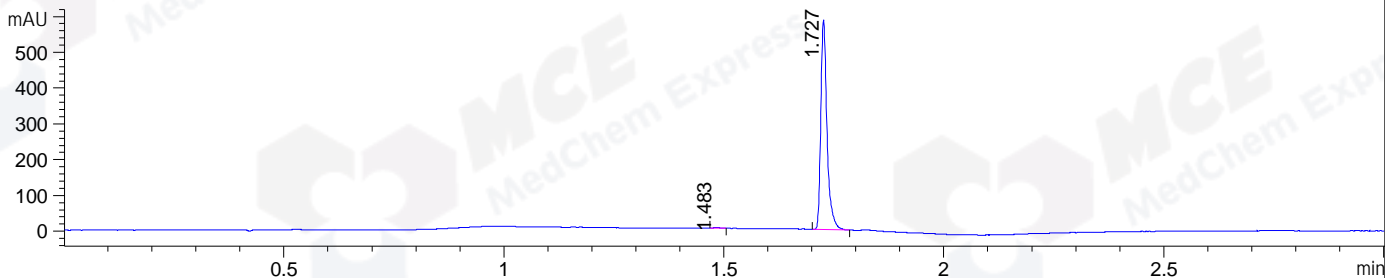

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

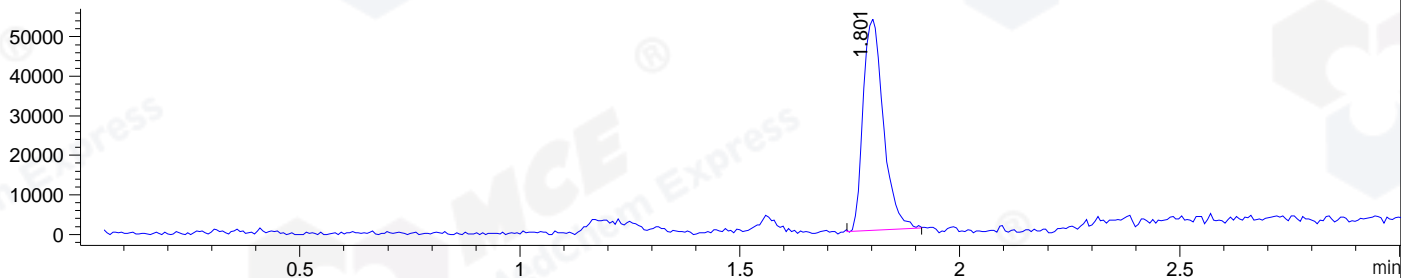

Ion 345, MSD1 345, Target Mass 344 +H Positive, EIC=344.7:345.7

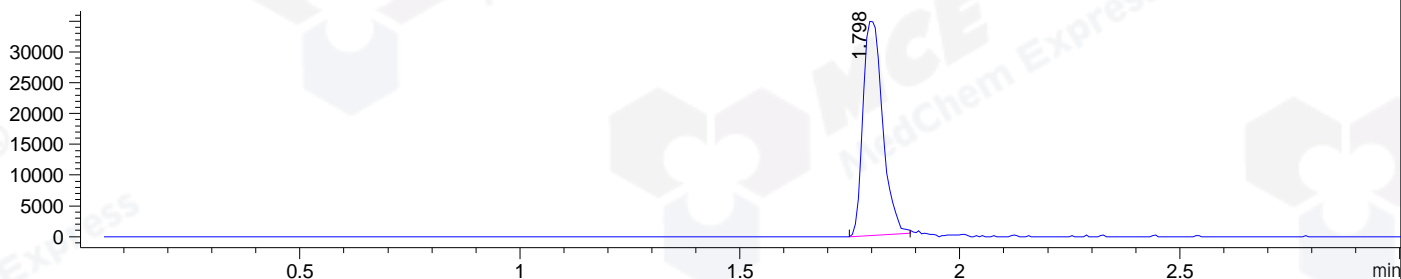

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.48	0.02	2.59	2.61	0.45	ND
1.73	0.02	574.50	586.37	99.55	345

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.80	0.05	172228.02	53411.18	100.00	345

Ret. Time: 1.80

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

