
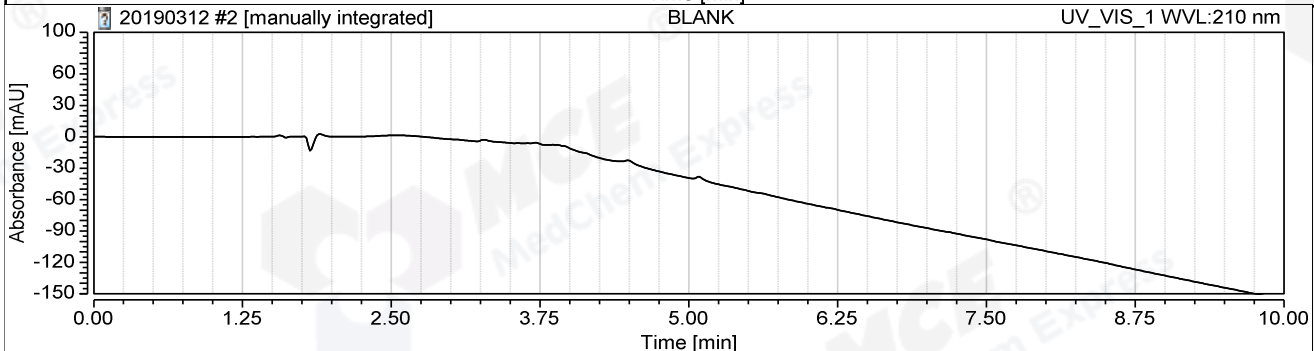


Chromatogram and Results

Injection Details

Injection Name:	BLANK	Injection Volume:	5.00
Vial Number:	RC8	Channel:	UV_VIS_1
Injection Type:	Unknown	Wavelength:	210
Calibration Level:		Users:	zqq
Instrument Method:	30-90A 210NM	Dilution Factor:	1.0000
Processing Method:	New Processing Method	Sample Weight:	1.0000
Injection Date/Time:	12/Mar/19 14:35		
Catalog No:	HY-19318 Batch#18668 A-RP-301		
chrom://hy261/ChromeleonLocal/Chemistry Analy/201903/20190312.seq/867.smp/UV_VIS_1.channel/UV_VIS_1.chm			

Chromatogram

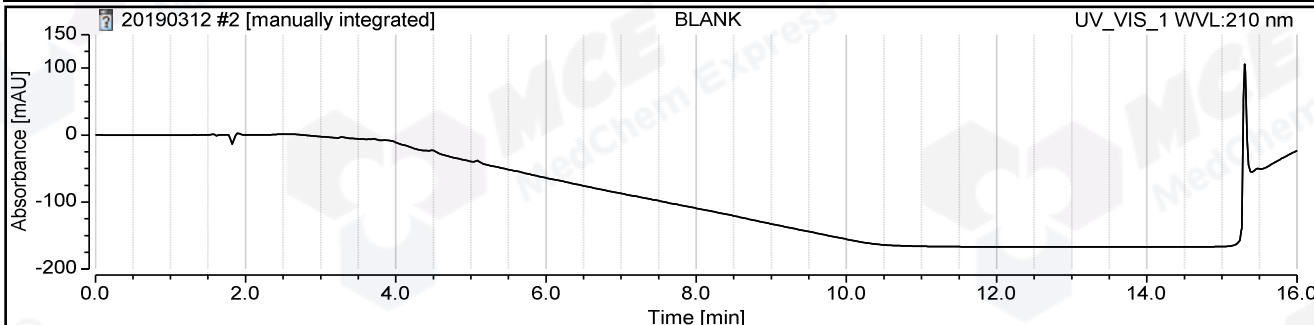

Integration Results



No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Asymmetry (EP)	Resolution (EP)	Rel.Area %
Total:			0.000	0.000	0.00	0.00	

Chromatogram and Results

Injection Details

Injection Name:	CPK2019-312-18668	Injection Volume:	5.00
Vial Number:	RD1	Channel:	UV_VIS_1
Injection Type:	Unknown	Wavelength:	210
Calibration Level:		Users:	zqq
Instrument Method:	30-90A 210NM	Dilution Factor:	1.0000
Processing Method:	New Processing Method	Sample Weight:	1.0000
Injection Date/Time:	12/Mar/19 14:52		
Catalog No:	HY-19318 Batch#18668 A-RP-301		
chrom://hy261/ChromeleonLocal/Chemistry Analy/201903/20190312.seq/211.smp/UV_VIS_1.channel/UV_VIS_1.chm			

Chromatogram

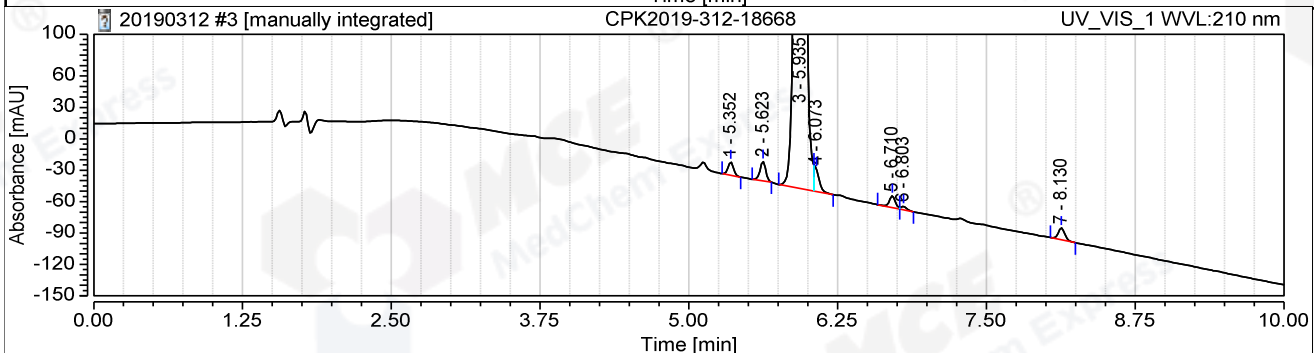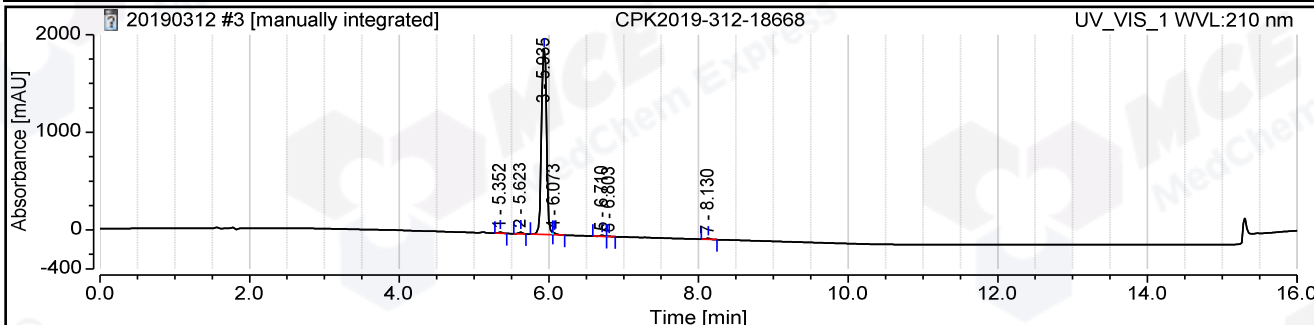

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Asymmetry (EP)	Resolution (EP)	Rel.Area %
1		5.352	0.675	12.679	1.05	3.21	0.44
2		5.623	1.032	18.561	0.93	2.95	0.67
3		5.935	150.098	1891.137	1.00	n.a.	97.15
4		6.073	1.133	21.585	n.a.	n.a.	0.73
5		6.710	0.664	11.337	n.a.	1.01	0.43
6		6.803	0.176	3.254	n.a.	13.70	0.11
7		8.130	0.716	11.223	1.11	n.a.	0.46
Total:			154.494	1969.776	4.09	20.88	