


3 CPK2019-110-19325**Catalog No: HY-19696A Batch#19325 A-RP-301 GWW**

Sample Name:	CPK2019-110-19325	Injection Volume:	100.0
Vial Number:	BA2	Channel:	UV_VIS_1
Sample Type:	unknown	Wavelength:	214
Control Program:	10-90A 214NM	Bandwidth:	n.a.
Quantif. Method:	default	Dilution Factor:	1.0000
Recording Time:	2019-1-11 9:17	Sample Weight:	1.0000
Run Time (min):	16.00	Sample Amount:	1.0000

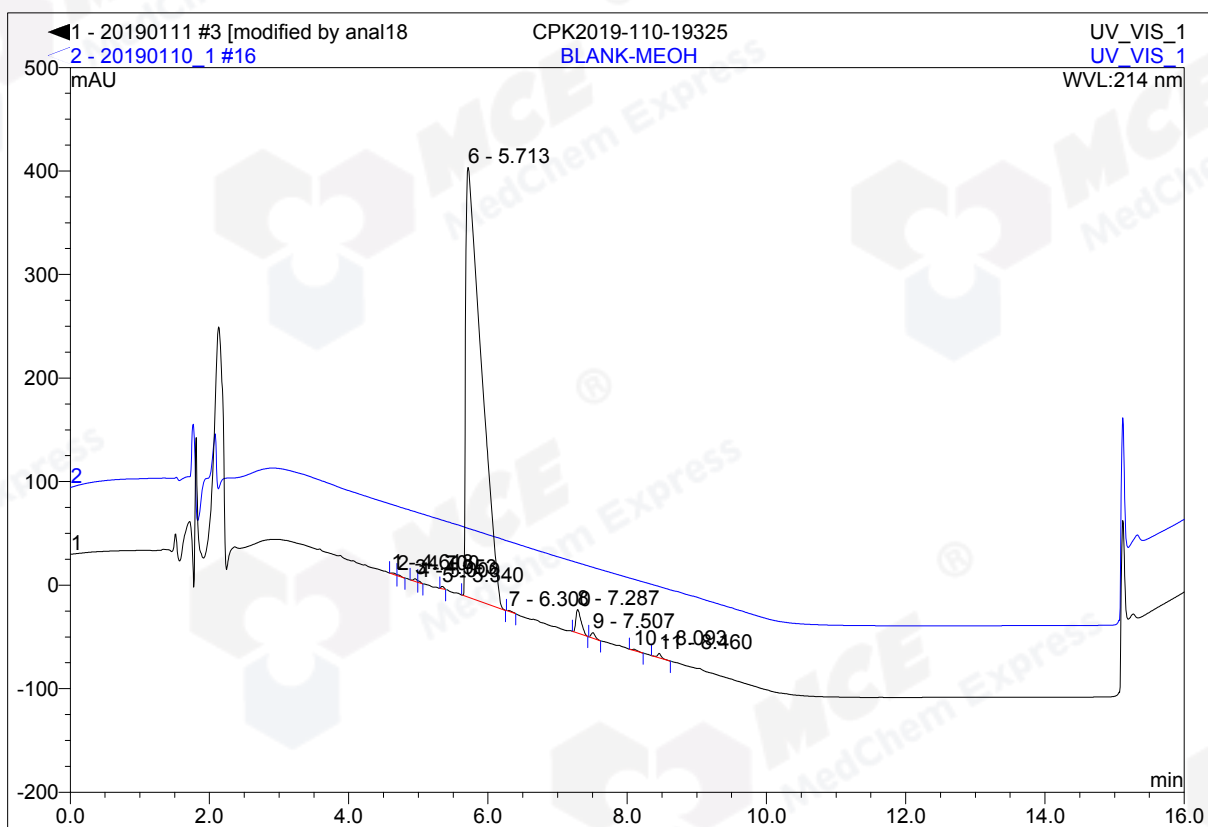

No.	Ret.Time min	Peak Name	Height mAU	Area mAU*min	Rel.Area %	Amount	Type
1	4.61	n.a.	0.718	0.093	0.08	n.a.	BM *
2	4.70	n.a.	0.707	0.059	0.05	n.a.	MB*
3	4.95	n.a.	2.425	0.142	0.13	n.a.	BM *
4	5.00	n.a.	1.380	0.063	0.06	n.a.	MB*
5	5.34	n.a.	2.366	0.112	0.10	n.a.	BMB*
6	5.71	n.a.	414.910	107.739	97.07	n.a.	BMB*
7	6.30	n.a.	0.735	0.066	0.06	n.a.	BMB*
8	7.29	n.a.	22.860	1.979	1.78	n.a.	BMB
9	7.51	n.a.	5.232	0.363	0.33	n.a.	BMB
10	8.09	n.a.	1.151	0.097	0.09	n.a.	BMB
11	8.46	n.a.	4.309	0.274	0.25	n.a.	BMB
Total:			456.793	110.987	100.00	0.000	