

File ..\DATA\2019\20190218\544\CPK2019-215-21382.D Tgt Mass (CHM):

Injection Date : 18 Feb 19 12:11 pm +0800 Seq. Line : 11

Sample Name : CPK2019-215-21382 Location : P1-B-07

Acq. Operator : LQ_1052 Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\Chem32\1\data\2019\20190218\544\1-POS-3MIN-1.M

Analysis Method : D:\CHEM32\1\DATA\2019\20190218\544\1-POS-3MIN-1.M

Catalog No : HY-19734 Batch#21382

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-314

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

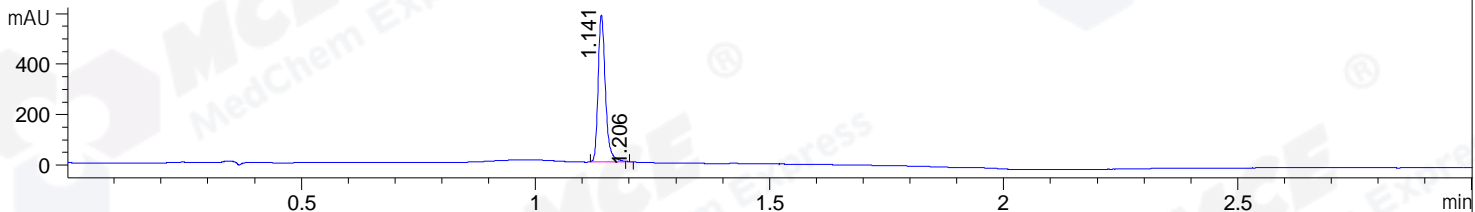


DAD1 C, Sig=254,4 Ref=off

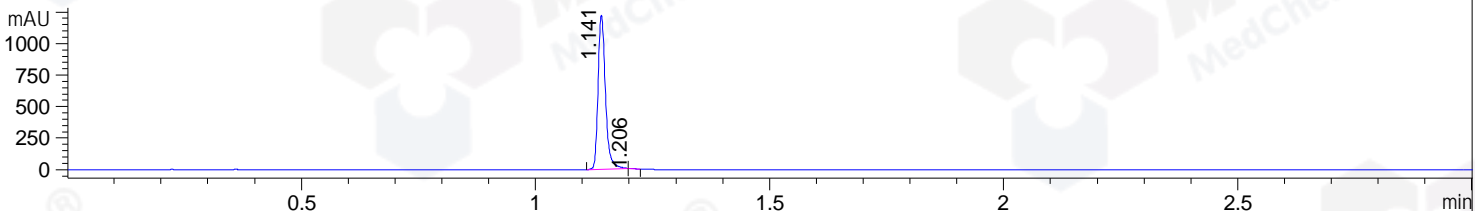

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

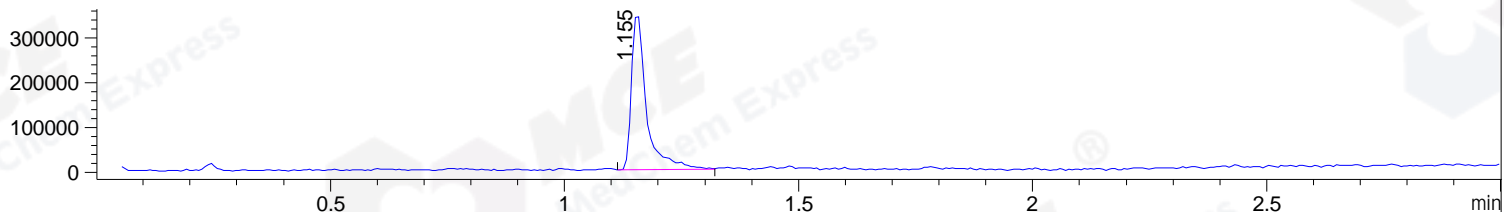

Ion 286.3, MSD1 286.3, Target Mass 285.3 +H Positive, EIC=286:287

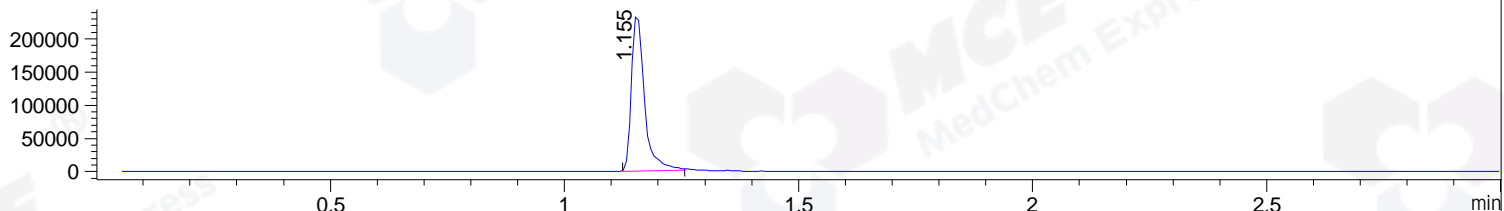

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.14	0.02	635.09	582.61	99.96	286
1.21	0.01	0.28	0.73	0.04	286

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.14	0.02	1345.39	1222.73	99.80	286
1.21	0.02	2.64	2.42	0.20	286

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.16	0.03	776670.63	350821.34	100.00	286

Ret. Time: 1.16

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

