



### Chromatogram and Results

#### Injection Details

Injection Name:	BLANKCPK2021-316-29931	Injection Volume:	2.00
Vial Number:	BA2	Channel:	UV_VIS_1
Injection Type:	Unknown	Wavelength:	214
Calibration Level:		Users:	zx
Instrument Method:	10-90A,214NM	Dilution Factor:	1.0000
Processing Method:	New Processing Method	Sample Weight:	1.0000
Injection Date/Time:	17/Mar/21 11:33	Run Time (min):	16.00
CAS NO.:	118-90-1 A-RP-757		

chrom://hy261/Themo/Instrument Data/202103/20210317.seq/140.smp/UV\_VIS\_1.channel/UV\_VIS\_1.chm

#### Chromatogram

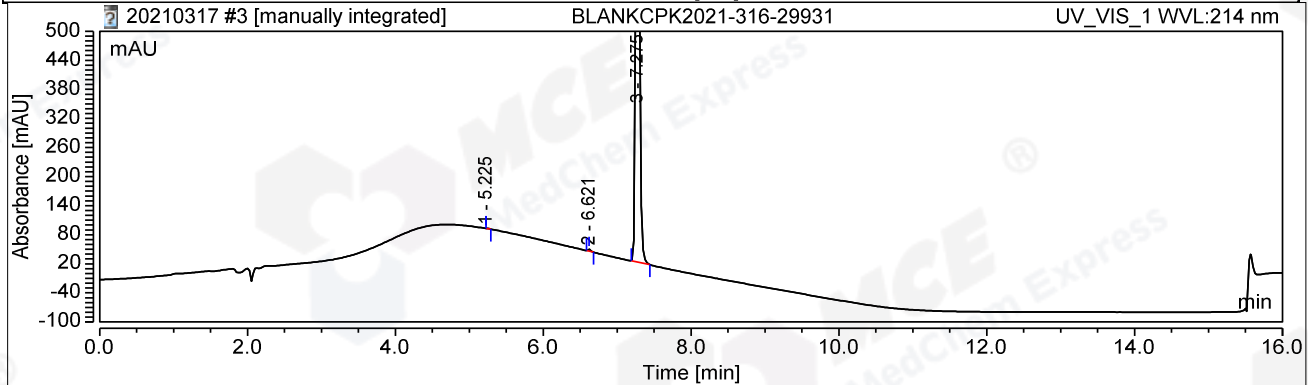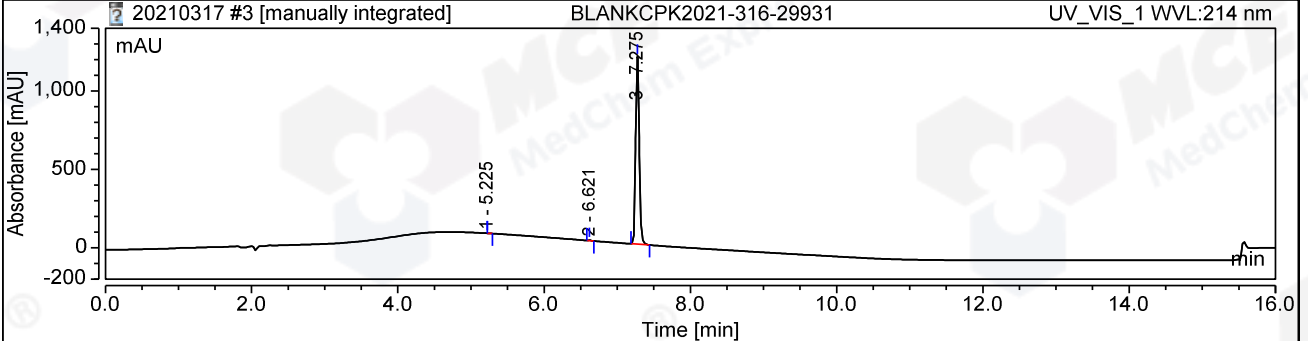

#### Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Asymmetry (EP)	Plates (EP)	Rel.Area %
1		5.225	0.021	0.000	n.a.	n.a.	0.03
2		6.621	0.178	4.118	1.27	144138	0.26
3		7.275	67.864	1193.882	1.16	105918	99.71
Total:			68.063	1198.000	2.42		