

File ..\DATA\2020\20200310\866\CPK2020-309-25346.D Tgt Mass (CHM):

Injection Date : 10 Mar 20 3:28 pm +0800 Seq. Line : 23

Sample Name : CPK2020-309-25346 Location : P1-D-05

Acq. Operator : ZJ_1432 Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\Chem32\1\data\2020\20200310\866\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2020\20200310\866\1-POS-3MIN.M

Catalog No : HY-50108 Batch#25346

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-433

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

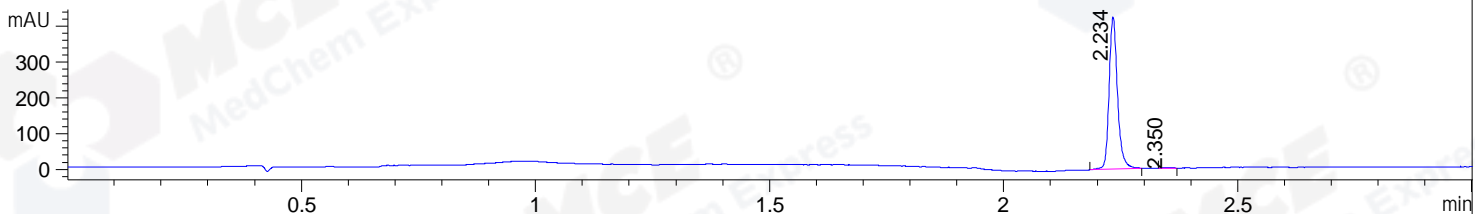


DAD1 C, Sig=254,4 Ref=off

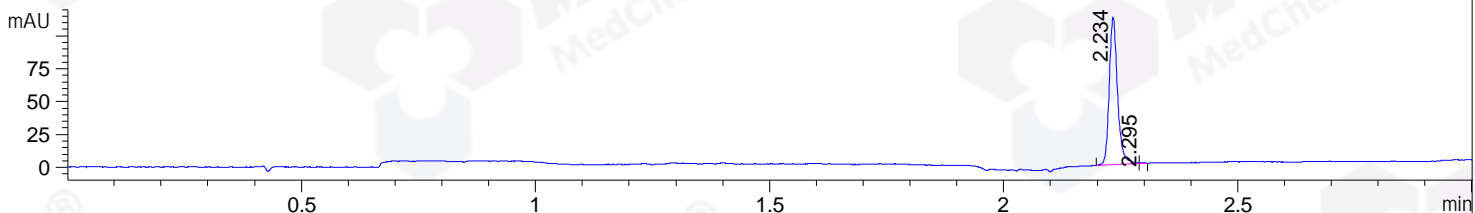

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

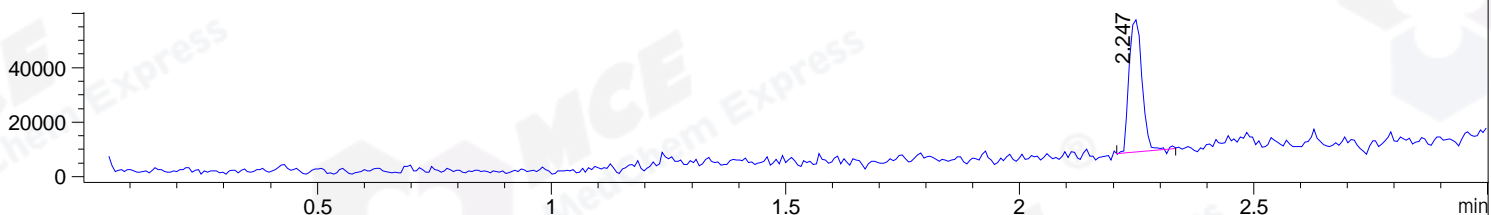

Ion 542, MSD1 542, Target Mass 541 +H Positive, EIC=541.7:542.7

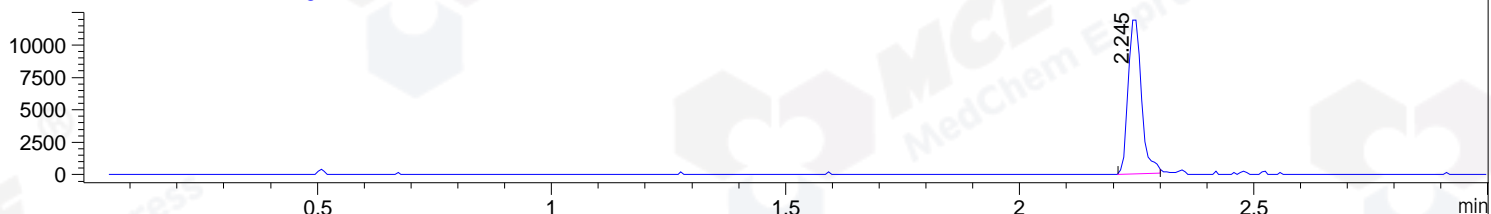

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
2.23	0.02	529.04	425.15	99.76	544
2.35	0.02	1.29	1.02	0.24	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
2.23	0.02	138.35	112.30	99.69	544
2.30	0.01	0.43	0.66	0.31	140

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
2.25	0.03	94037.95	48942.23	100.00	544

Ret. Time: 2.25

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

