



File ..DATA\2019\20190712\629\CPK2019-711-19257-.D Tgt Mass (CHM):
Injection Date : 12 Jul 19 1:27 pm +0800 Seq. Line : 30
Sample Name : CPK2019-711-19257 Location : P1-C-09
Acq. Operator : ZJ_1432 Inj : 1
Spec. Reported : MS Integration Inj Volume : 0.4 ul
Acq. Method : D:\Chem32\1\data\2019\20190712\629\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2019\20190712\629\1-POS-3MIN.M
Catalog No : HY-50862 Batch#19257
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

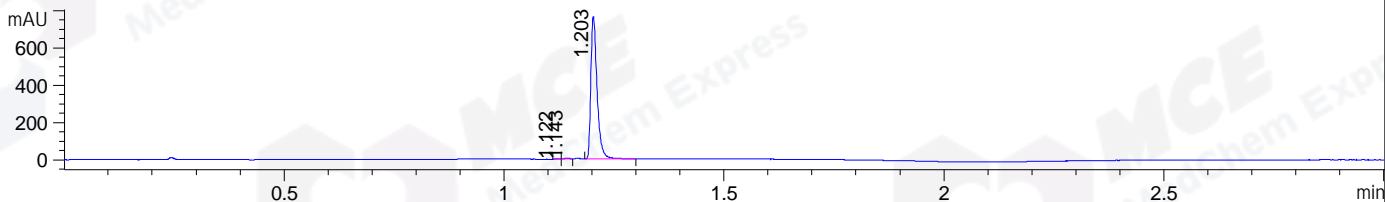


DAD1 C, Sig=254,4 Ref=off

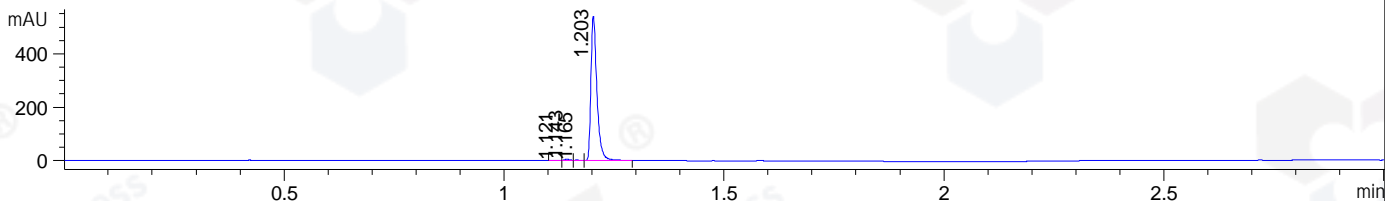

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

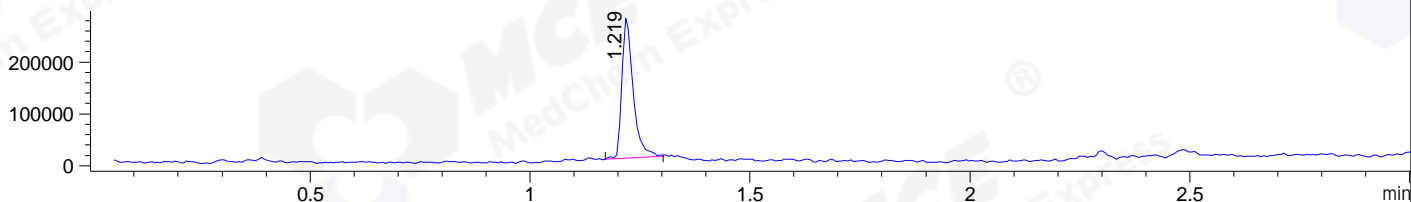

Ion 540.6454, MSD1 540.6454, Target Mass 539.6454 +H Positive, EIC=540.35:541.35

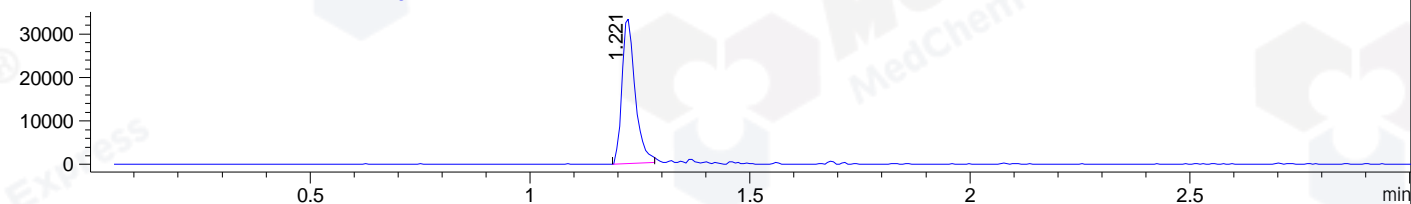

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.12	0.01	1.07	1.73	0.14	ND
1.14	0.01	5.21	6.22	0.69	ND
1.20	0.02	751.14	764.87	99.17	271

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.12	0.01	1.10	1.40	0.21	220
1.14	0.01	4.20	4.69	0.81	ND
1.17	0.01	1.83	2.06	0.35	390
1.20	0.02	509.69	541.44	98.62	271

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.22	0.03	486217.66	274678.56	100.00	271

Ret. Time: 1.22

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

