



File ..DATA\2020\20200225\851\CPK2020-224-16369-.D Tgt Mass (CHM):
 Injection Date : 25 Feb 20 2:45 pm +0800 Seq. Line : 64
 Sample Name : CPK2020-224-16369 Location : P1-B-01
 Acq. Operator : ZJ_1432 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 0.5 ul
 Acq. Method : D:\Chem32\1\data\2020\20200225\851\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200225\851\1-POS-3MIN.M
 Catalog No : HY-66005 Batch#16369
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

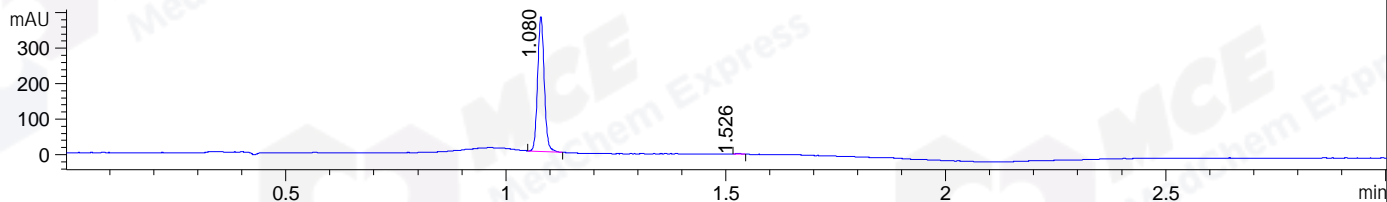


DAD1 C, Sig=254,4 Ref=off

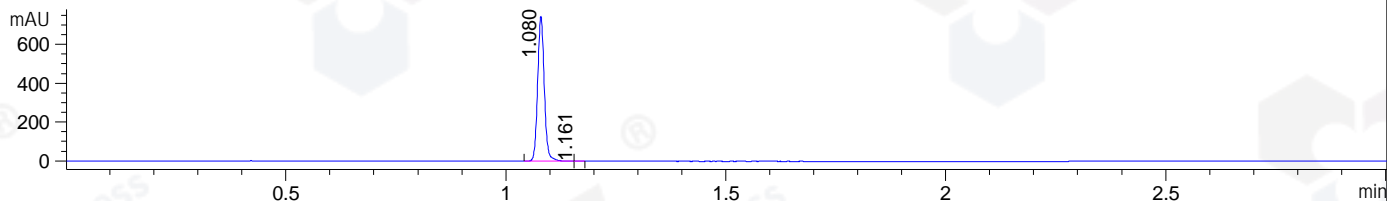

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

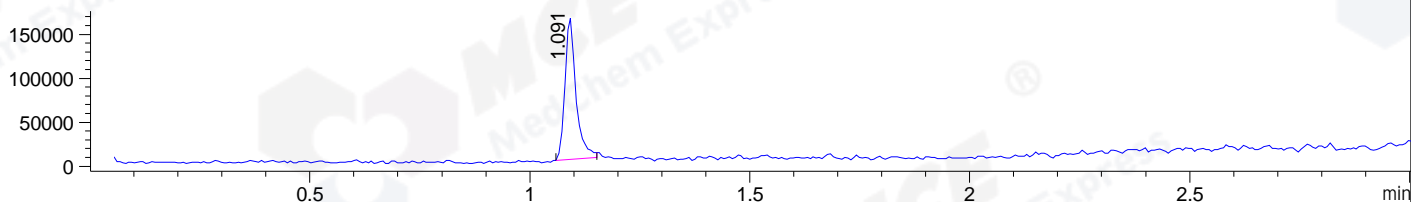

Ion 152, MSD1 152, Target Mass 151 +H Positive, EIC=151.7:152.7

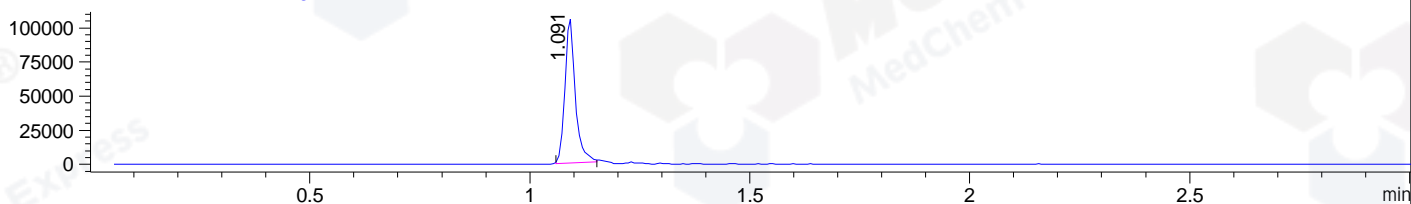

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.08	0.02	399.12	380.64	99.53	152
1.53	0.02	1.88	1.98	0.47	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.08	0.02	784.20	746.43	99.96	152
1.16	0.02	0.33	0.36	0.04	152

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.09	0.03	284225.28	162984.83	100.00	152

Ret. Time: 1.09

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

