



File ..ATA\2020\20200811\1066\CPK2020-810-15664-.D Tgt Mass (CHM):
Injection Date : 12 Aug 20 12:23 am +0800 Seq. Line : 127
Sample Name : CPK2020-810-15664 Location : P1-C-02
Acq. Operator : ZJ_1432 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2020\20200811\1066\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20200811\1066\1-POS-3MIN.M
Catalog No : HY-66009
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-607
Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

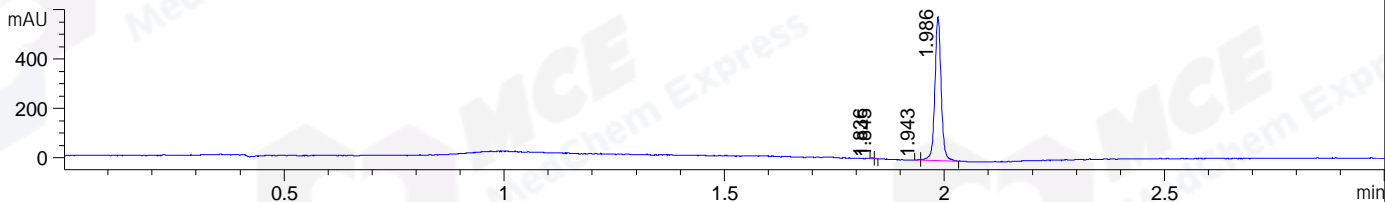


DAD1 C, Sig=254,4 Ref=off

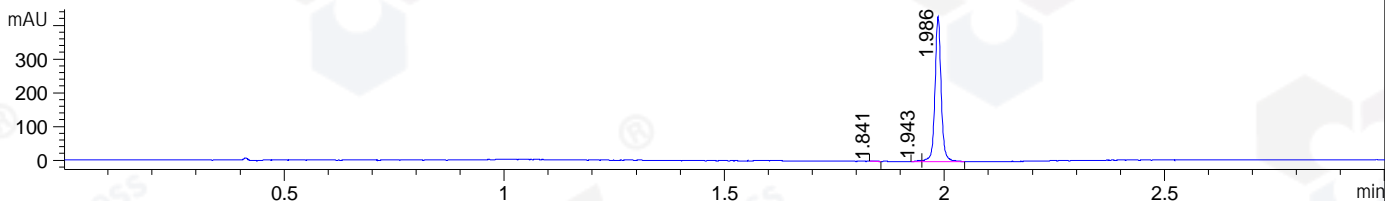

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

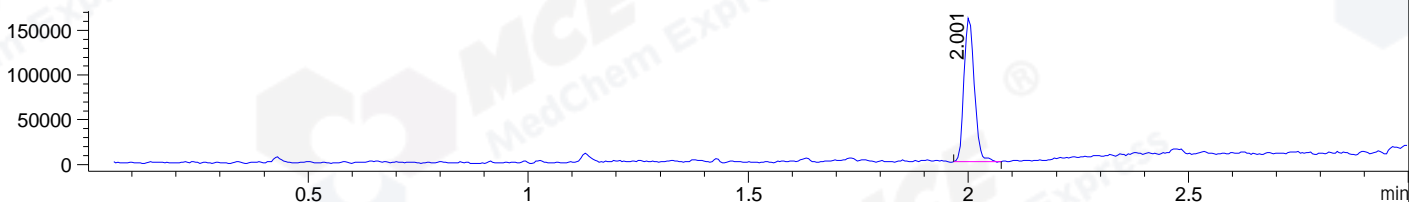

Ion 320, MSD1 320, Target Mass 319 +H Positive, EIC=319.7:320.7

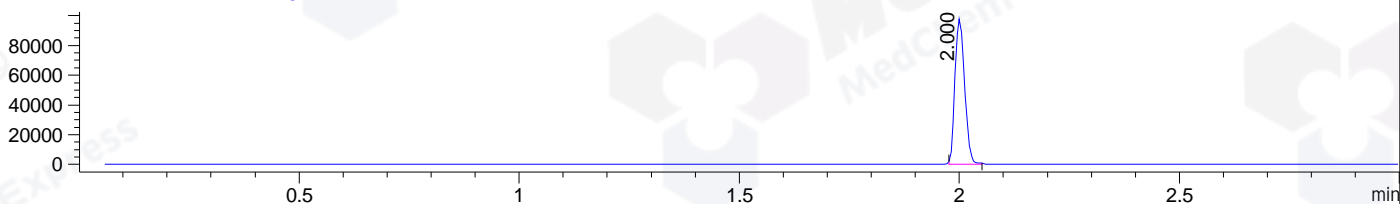

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.84	0.01	0.66	2.05	0.11	ND
1.84	0.01	0.59	1.92	0.10	ND
1.94	0.01	1.12	2.48	0.19	ND
1.99	0.02	580.42	584.48	99.59	320

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.84	0.01	1.32	1.48	0.31	ND
1.94	0.01	2.70	3.29	0.63	ND
1.99	0.02	423.46	431.38	99.06	320

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
2.00	0.03	264345.53	161508.31	100.00	320

Ret. Time: 2.00

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

