



File ..DATA\2020\20200921\1112\CPK2020-915-13760.D Tgt Mass (CHM):
 Injection Date : 21 Sep 20 11:42 am +0800 Seq. Line : 36
 Sample Name : CPK2020-915-13760 Location : P1-A-02
 Acq. Operator : zyj_1547 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20200921\1112\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200921\1112\1-POS-3MIN.M
 Catalog No : HY-A0013
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-624


DAD1 B, Sig=214,4 Ref=off

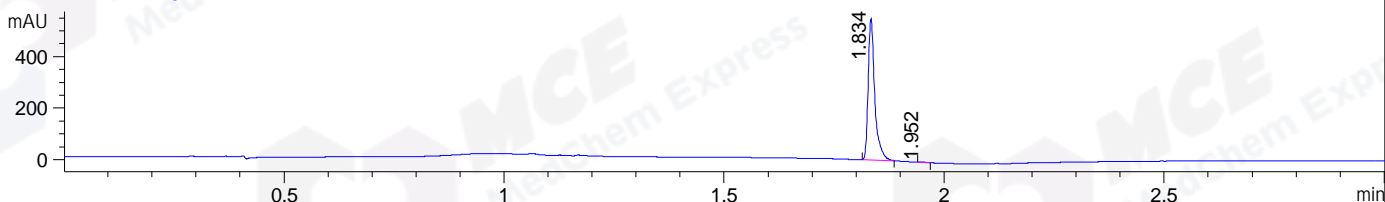


DAD1 C, Sig=254,4 Ref=off

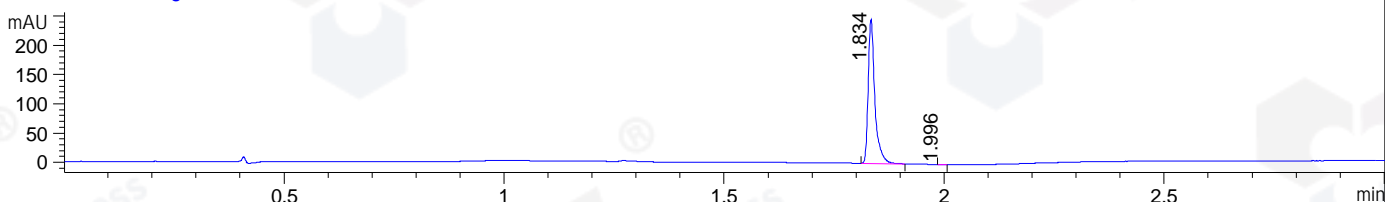

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

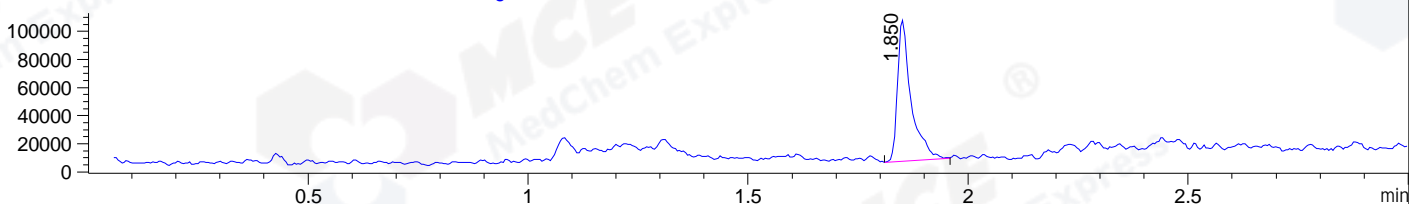

Ion 552, MSD1 552, Target Mass 551 +H Positive, EIC=551.7:552.7

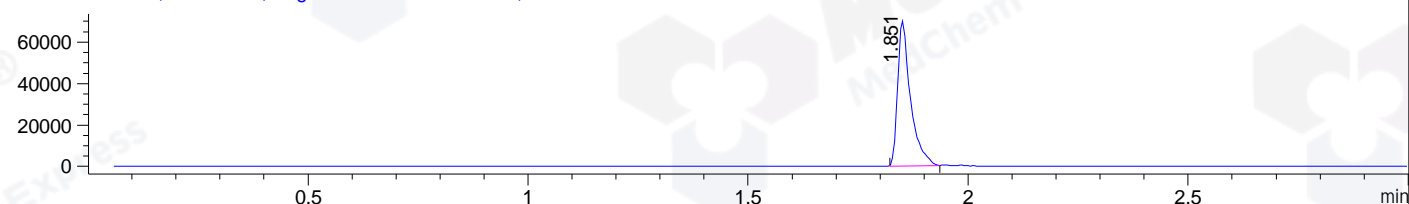

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.83	0.02	570.46	549.71	99.93	552
1.95	0.02	0.43	0.42	0.07	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.83	0.02	258.13	246.26	99.92	552
2.00	0.01	0.21	0.33	0.08	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.85	0.03	219193.66	100832.40	100.00	552

Ret. Time: 1.85

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

