

File ..Data\20170905\20170905-1\BIZ2017-905-WYQ6.D Tgt Mass (CHM):

Injection Date : 5 Sep 17 12:14 pm +0800 Seq. Line : 17

Sample Name : BIZ2017-905-WYQ6 Location : P1-C-04

Acq. Operator : SYSTEM Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\LCMS03\Data\20170905\20170905-1\1-POS-3MIN.M

Analysis Method : D:\LCMS03\Data\20170905\20170905-1\1-POS-3MIN.M

Catalog No : HY-A0098 Batch#26163

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-186

Oven Temperature : 45C


DAD1 A, Sig=214,4 Ref=off

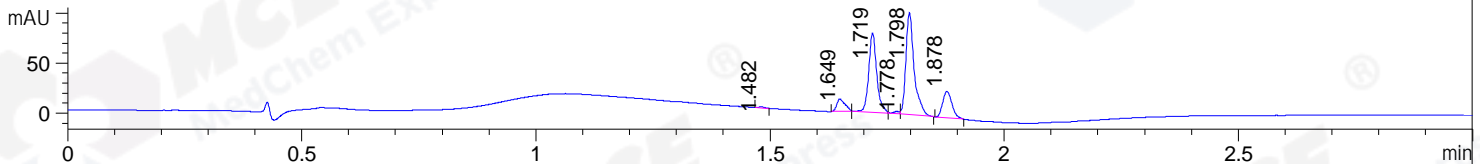


DAD1 B, Sig=254,4 Ref=off

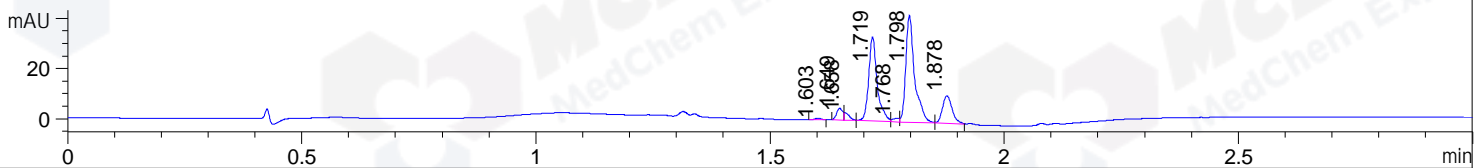


ELS1 A, ELSD Signal

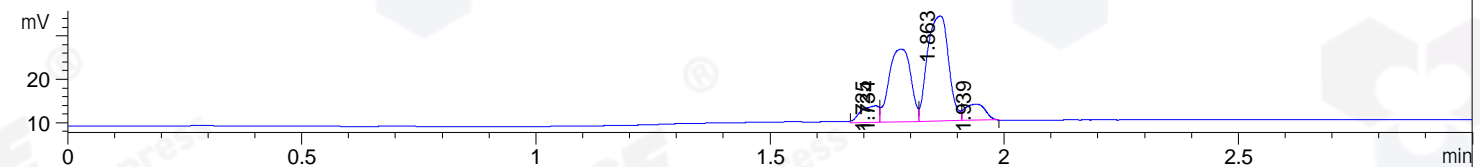

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

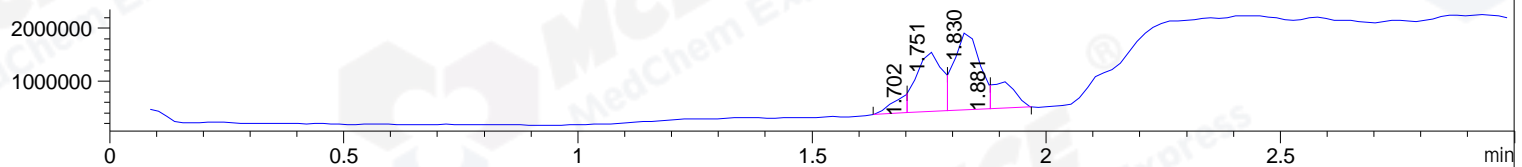

Ion 704.2, MSD1 704.2, Target Mass 704.2 Positive, EIC=703.9:704.9

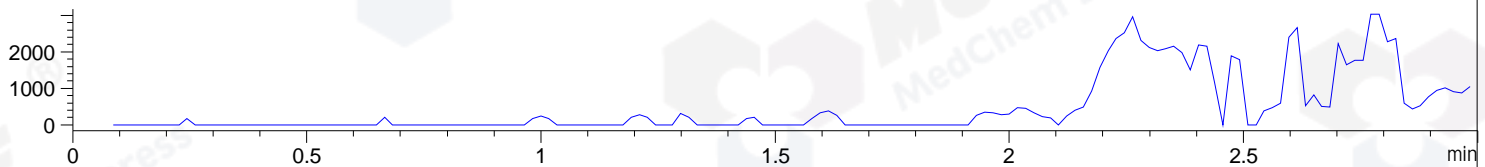

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.48	0.02	1.21	1.17	0.44	214
1.65	0.02	15.37	12.45	5.59	596
1.72	0.02	94.62	79.63	34.39	610
1.78	0.01	2.04	2.32	0.74	610
1.80	0.02	125.25	102.15	45.52	624
1.88	0.02	36.65	26.48	13.32	638


Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.60	0.02	0.53	0.58	0.43	105
1.65	0.02	4.24	4.64	3.46	105
1.66	0.01	2.29	3.06	1.87	596
1.72	0.02	42.69	33.58	34.81	610
1.77	0.02	1.37	1.36	1.11	610
1.80	0.02	55.81	42.54	45.51	624
1.88	0.02	15.70	10.97	12.81	638


Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.70	0.05	1075074.13	342046.44	8.83	596
1.75	0.06	4273723.50	1151362.63	35.11	610
1.83	0.06	5433894.00	1503913.63	44.64	624
1.88	0.05	1389987.63	449829.75	11.42	638


Ret. Time: 1.70 <<<< POSITIVE SPECTRA >>>>

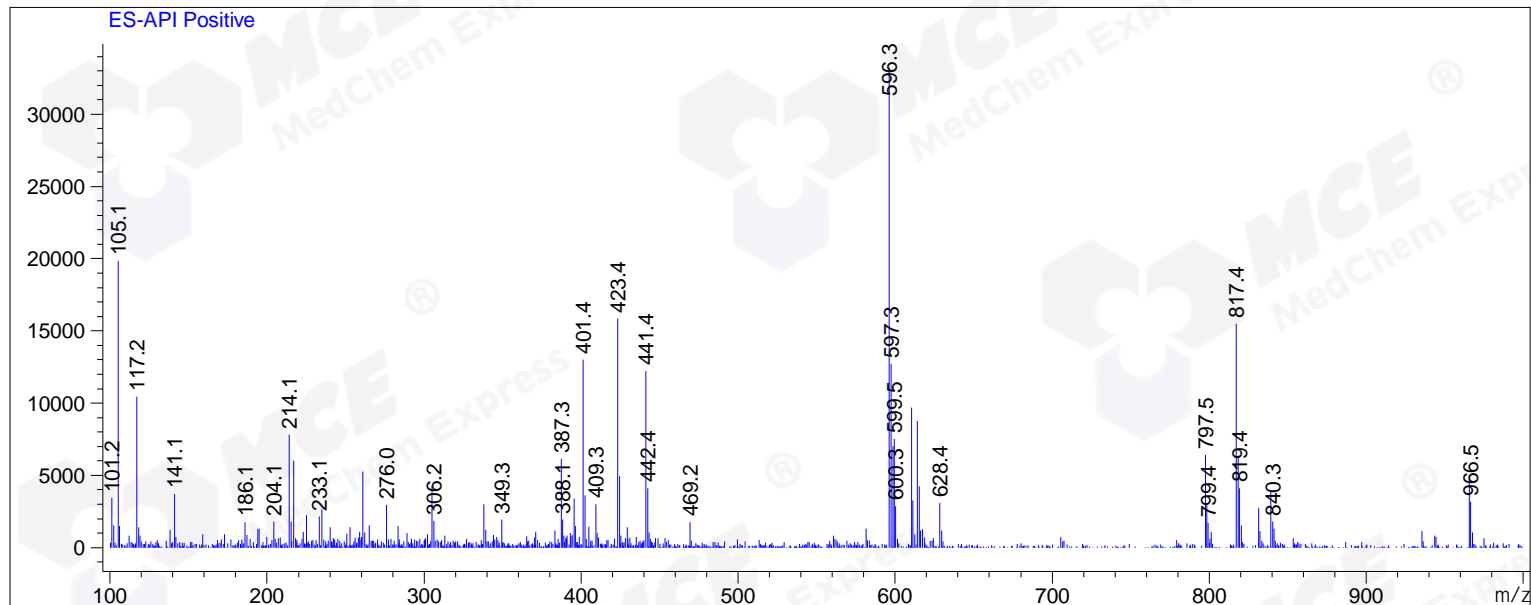


Ret. Time: 1.75

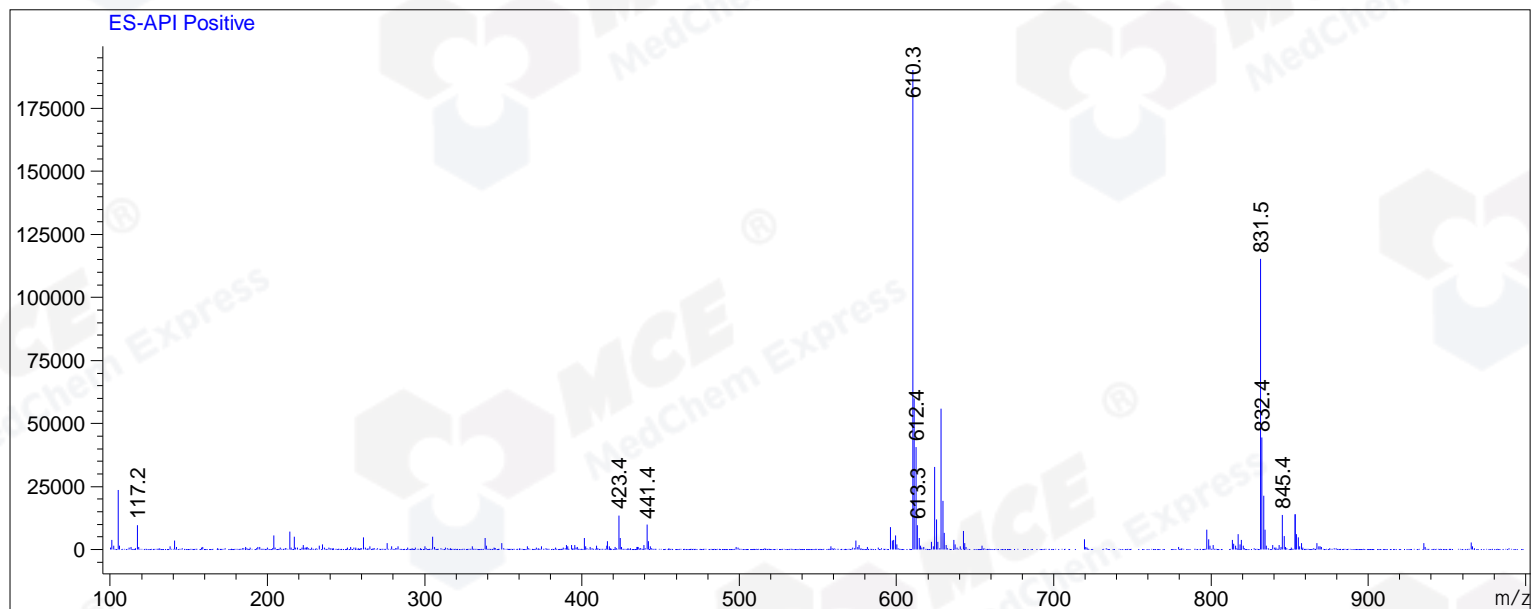

Ret. Time: 1.83

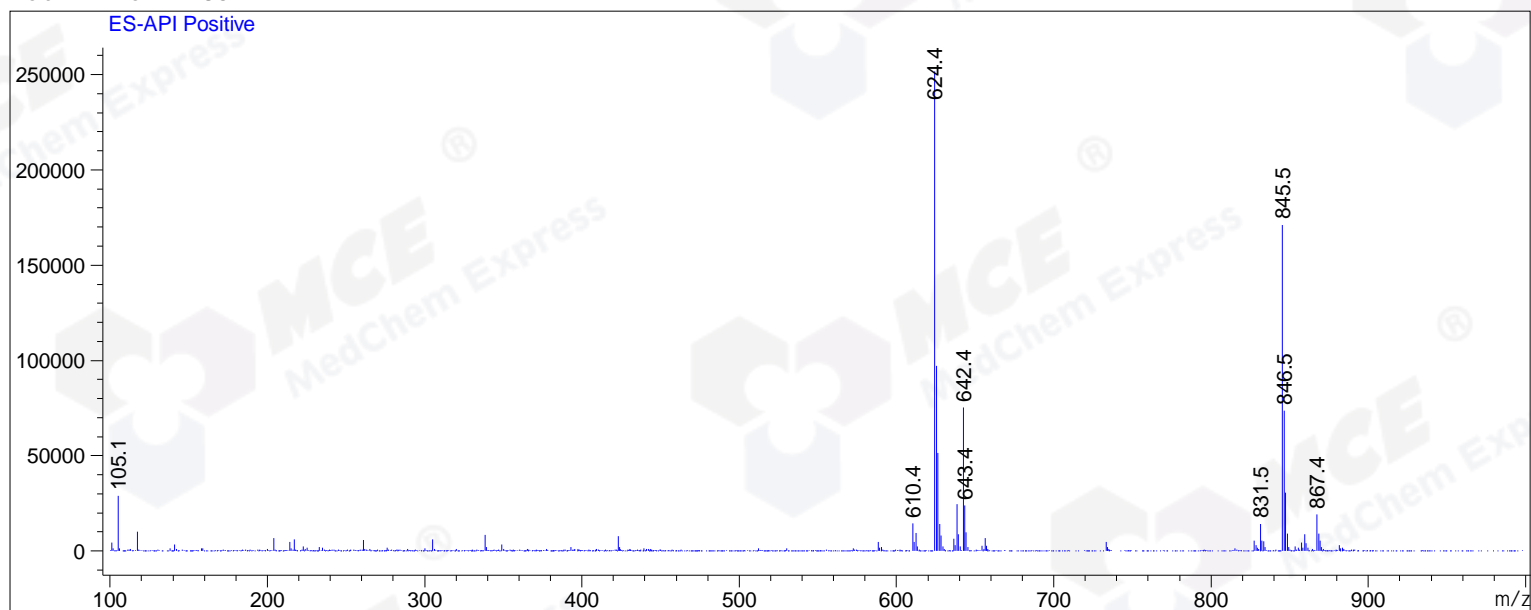

Ret. Time: 1.88

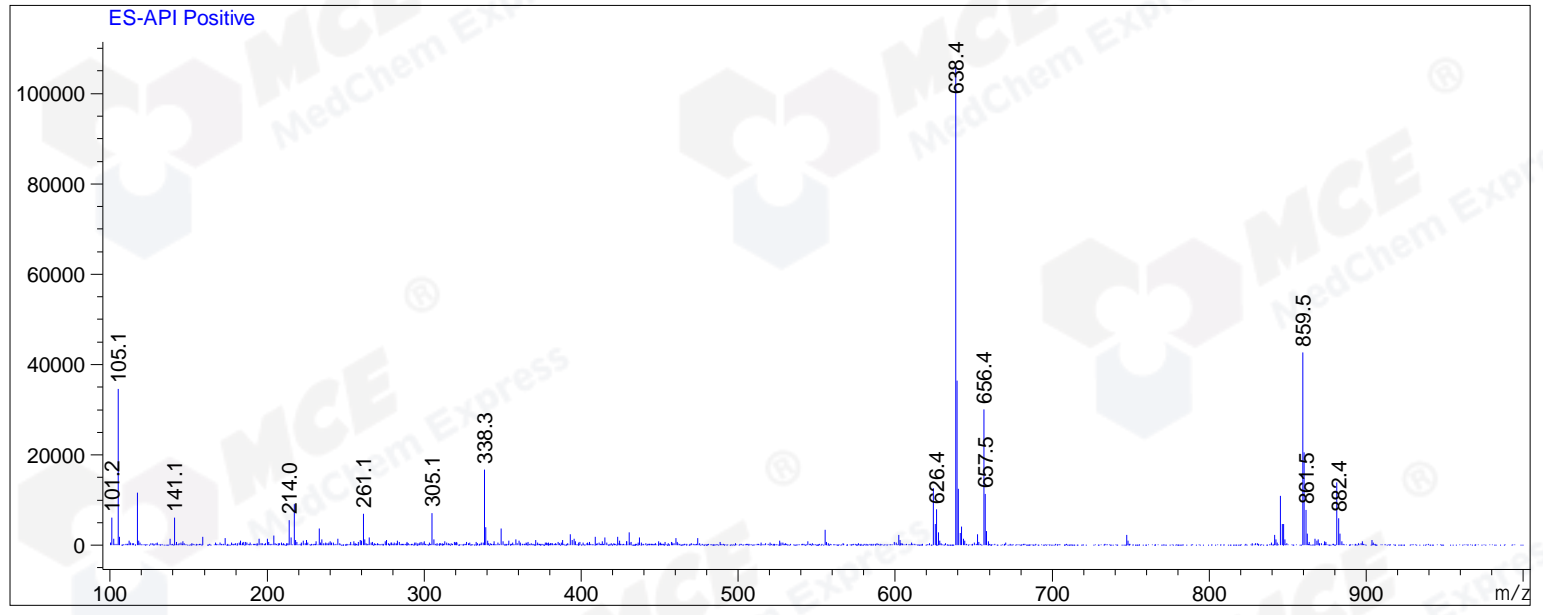

*** End of Report ***