



File ..DATA\2021\20210330\1319\CPK2021-329-32316.D Tgt Mass (CHM):
 Injection Date : 30 Mar 21 3:38 pm +0800 Seq. Line : 83
 Sample Name : CPK2021-329-32316 Location : P1-A-07
 Acq. Operator : yrz_1364 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2021\20210330\1319\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2021\20210330\1319\1-POS-3MIN.M
 CAS NO. : 53772-83-1
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

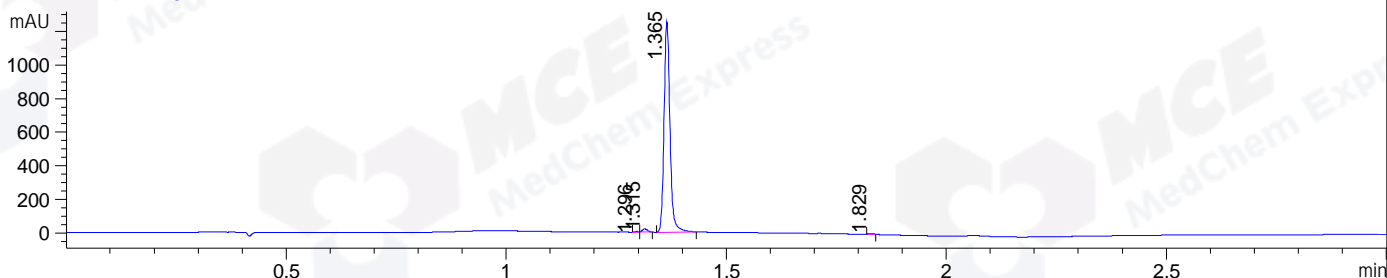

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

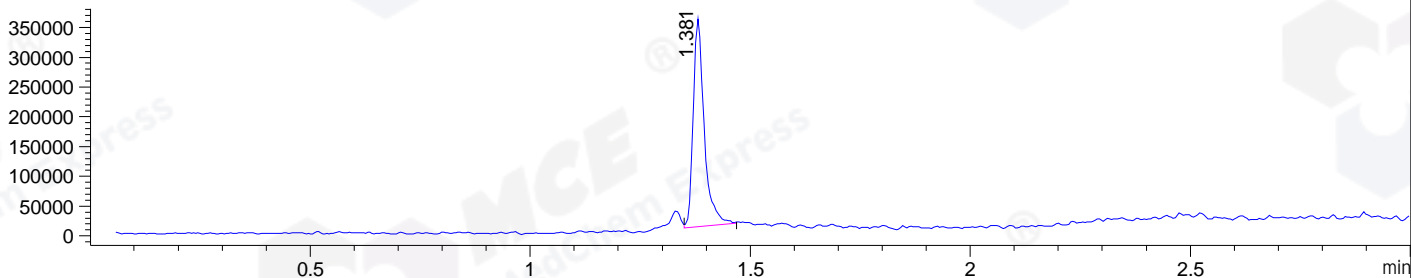

Ion 401, MSD1 401, Target Mass 400 +H Positive, EIC=400.7:401.7

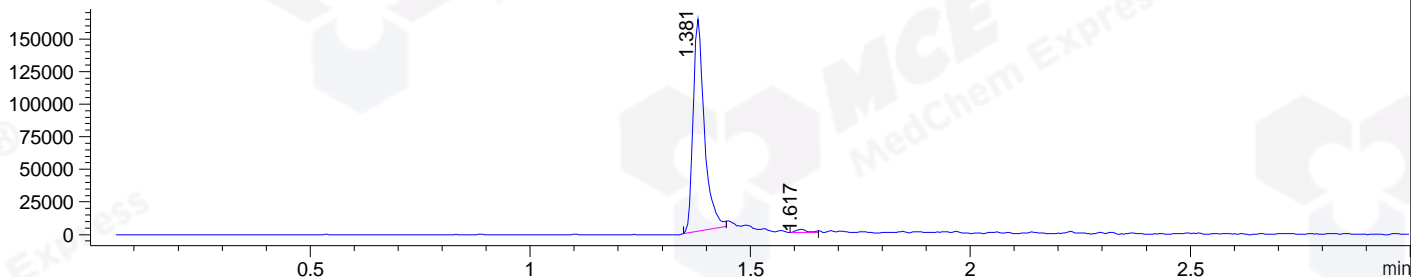

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.30	0.01	2.45	3.79	0.21	395
1.31	0.01	16.65	20.32	1.40	417
1.37	0.02	1171.13	1248.77	98.13	401
1.83	0.01	3.26	4.36	0.27	401

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.38	0.03	611900.81	348698.03	100.00	401

Ret. Time: 1.38

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

