



File ..\DATA\2019\20190520\583\BIZ2019-520-WYQ20.D Tgt Mass (CHM):
 Injection Date : 20 May 19 4:46 pm +0800 Seq. Line : 30
 Sample Name : BIZ2019-520-WYQ20 Location : P1-C-02
 Acq. Operator : LQ_1052 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 5 ul
 Acq. Method : D:\Chem32\1\data\2019\20190520\583\1-POS-3MIN-1(110-1500).M
 Analysis Method : D:\CHEM32\1\DATA\2019\20190520\583\1-POS-3MIN-1(110-1500).M
 Catalog No : HY-A0182 Batch#41278
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-314
 Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

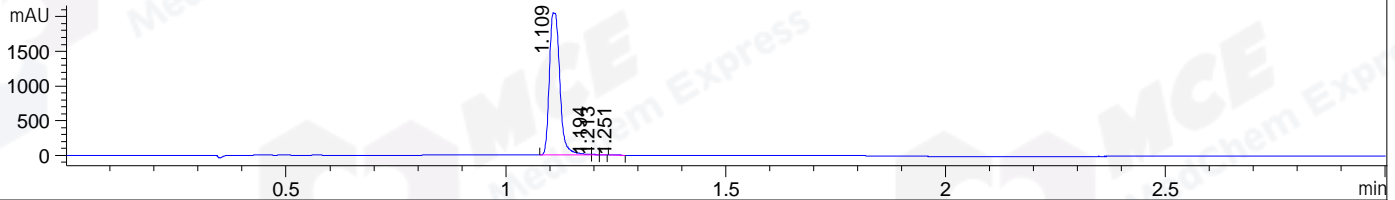


DAD1 C, Sig=254,4 Ref=off

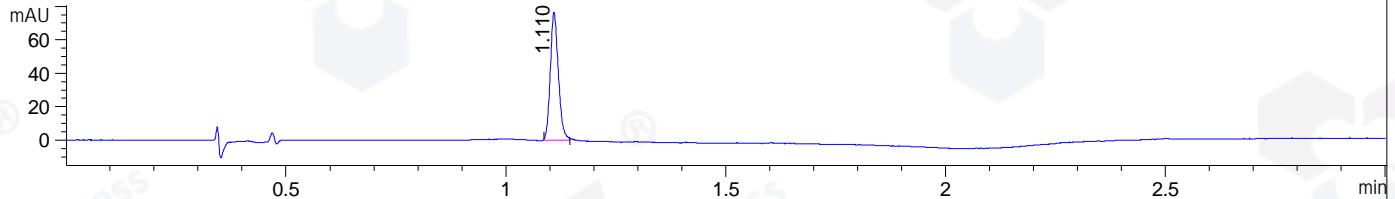

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

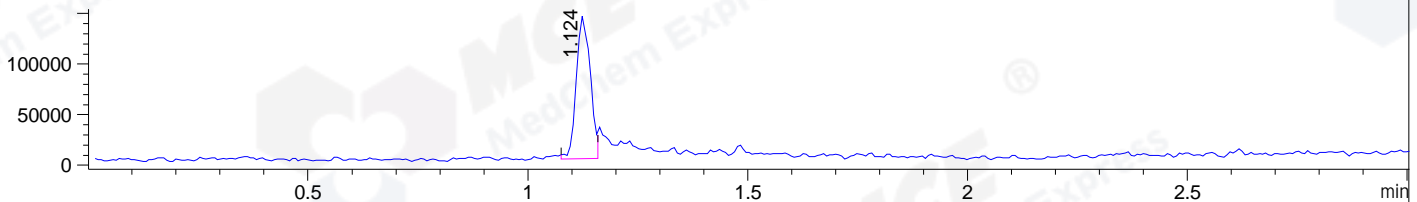

Ion 1040.4, MSD1 1040.4, Target Mass 1039.4 +H Positive, EIC=1040.1:1041.1

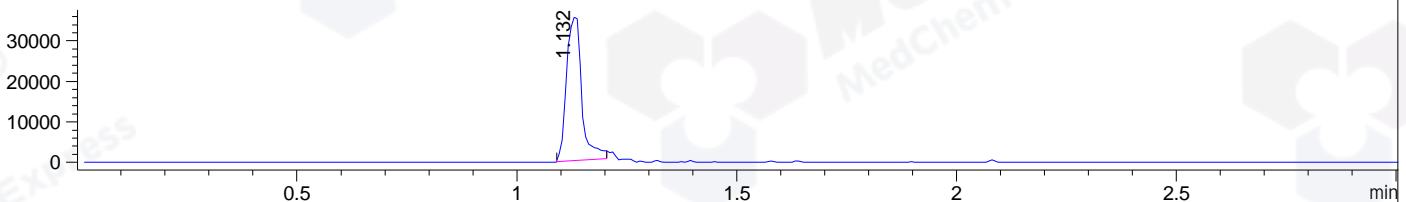

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.11	0.03	3379.44	2057.54	99.68	521
1.19	0.01	4.87	6.34	0.14	521
1.21	0.01	1.86	2.61	0.05	521
1.25	0.02	4.02	2.83	0.12	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.11	0.02	97.57	76.56	100.00	521

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.12	0.03	311531.53	141076.44	100.00	521

Ret. Time: 1.12

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

