



File ..TA\2020\20201210\1194\BIZ2020-D03-SCH5-1-.D Tgt Mass (CHM):
 Injection Date : 10 Dec 20 4:37 pm +0800 Seq. Line : 98
 Sample Name : BIZ2020-D03-SCH5-1 Location : P1-A-06
 Acq. Operator : zyj_1547 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 0.5 ul
 Acq. Method : D:\Chem32\1\data\2020\20201210\1194\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20201210\1194\1-POS-3MIN.M
 CAS NO. : 50-91-9
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

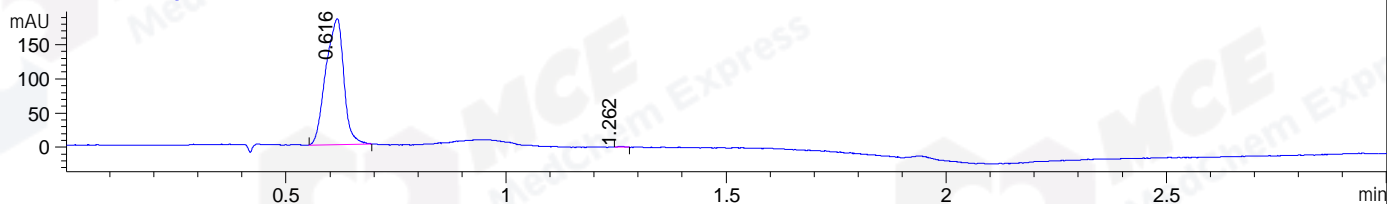


DAD1 C, Sig=254,4 Ref=off

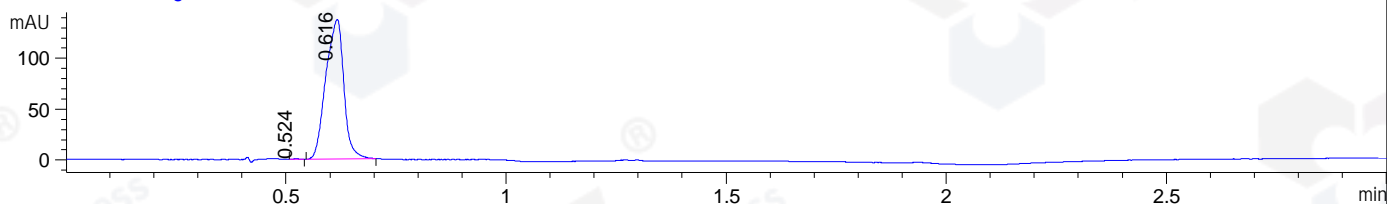

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

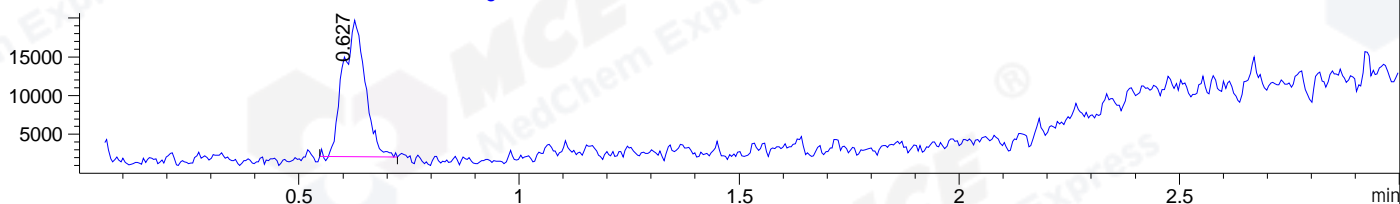

Ion 1, MSD1 1, Target Mass 0 +H Positive, EIC=0.7:1.7

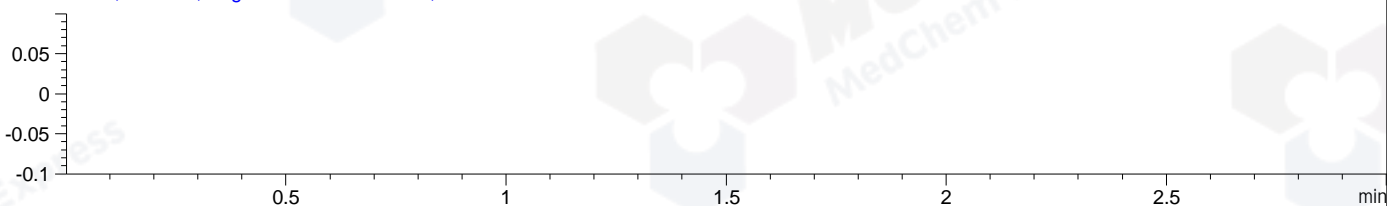

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
0.62	0.05	522.68	184.38	99.76	269
1.26	0.02	1.26	1.08	0.24	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
0.52	0.02	0.65	0.56	0.17	ND
0.62	0.05	390.01	137.39	99.83	269

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
0.63	0.05	61747.29	17647.86	100.00	269

Ret. Time: 0.63

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

