



File ..DATA\2020\20200314\872\CPK2020-313-14239-.D Tgt Mass (CHM):
Injection Date : 14 Mar 20 3:11 pm +0800 Seq. Line : 21
Sample Name : CPK2020-313-14239 Location : P1-B-03
Acq. Operator : ZJ_1432 Inj : 1
Spec. Reported : MS Integration Inj Volume : 0.5 ul
Acq. Method : D:\Chem32\1\data\2020\20200314\872\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20200314\872\1-POS-3MIN.M
Catalog No : HY-B0105 Batch#14239
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

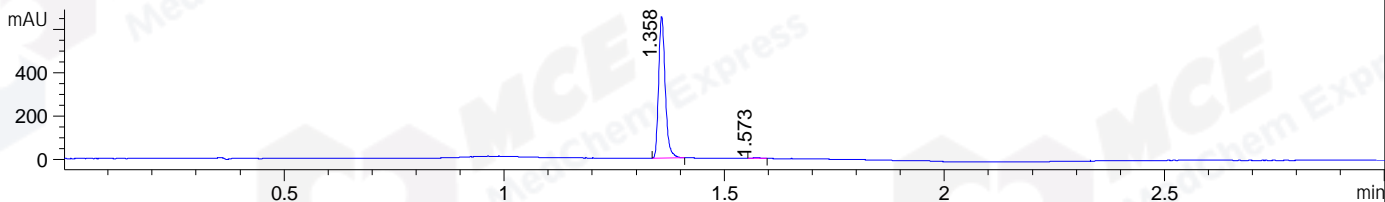


DAD1 C, Sig=254,4 Ref=off

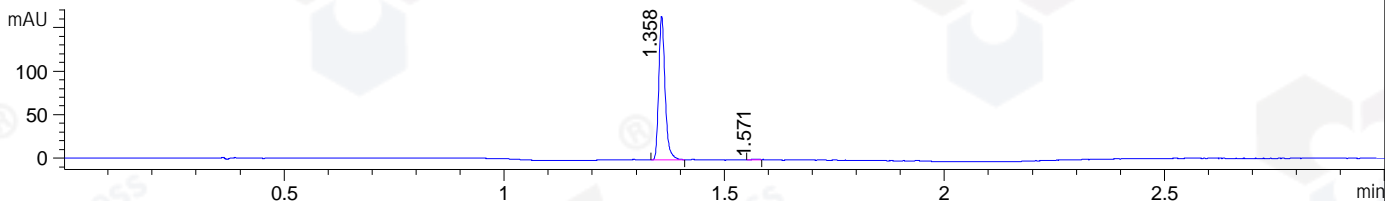

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

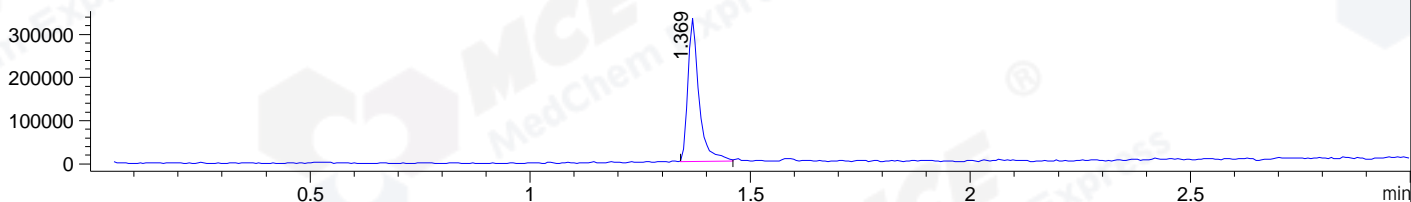

Ion 531, MSD1 531, Target Mass 530 +H Positive, EIC=530.7:531.7

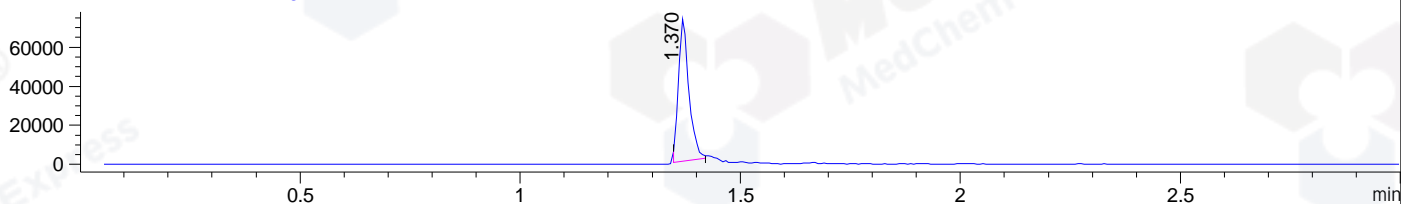

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.36	0.02	681.47	653.60	99.34	531
1.57	0.02	4.50	4.51	0.66	274

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.36	0.02	165.18	165.11	99.47	531
1.57	0.02	0.88	0.95	0.53	274

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.37	0.03	590025.75	332651.00	100.00	531

Ret. Time: 1.37

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

