



File ..\DATA\2020\20200509\950\CPK2020-508-15876.D Tgt Mass (CHM):  
 Injection Date : 9 May 20 3:07 pm +0800 Seq. Line : 81  
 Sample Name : CPK2020-508-15876 Location : P1-A-09  
 Acq. Operator : ZJ\_1432 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2020\20200509\950\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2020\20200509\950\1-POS-3MIN.M  
 Catalog No : HY-B0157A  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-607  
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

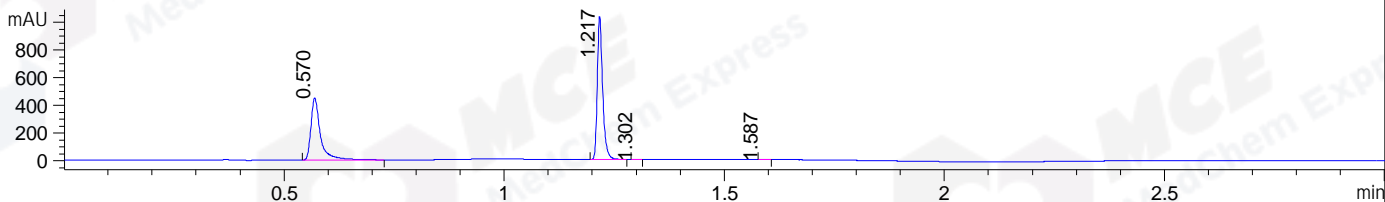


DAD1 C, Sig=254,4 Ref=off

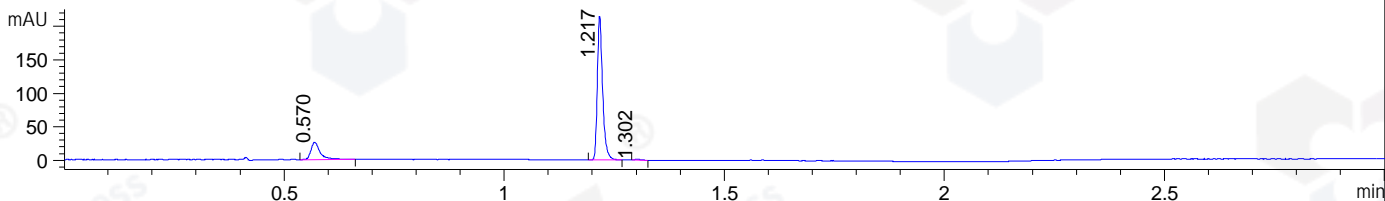

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

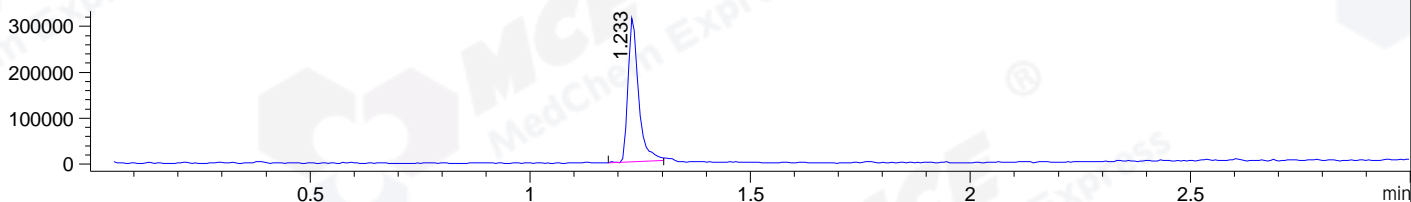

Ion 310, MSD1 310, Target Mass 309 +H Positive, EIC=309.7:310.7

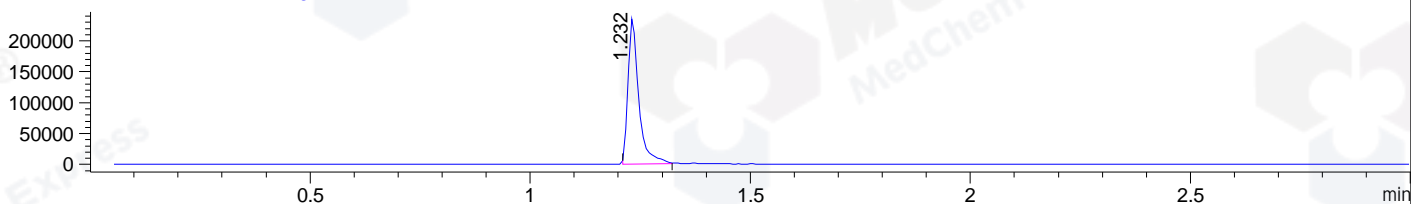

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
0.57	0.02	672.65	449.19	43.50	ND
1.22	0.01	871.09	1035.04	56.33	310
1.30	0.01	1.49	2.12	0.10	310
1.59	0.02	1.09	1.20	0.07	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
0.57	0.02	37.35	25.76	17.16	130
1.22	0.01	179.24	215.22	82.36	310
1.30	0.01	1.03	1.34	0.47	310

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.23	0.03	521929.94	318355.00	100.00	310

Ret. Time: 1.23

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

