
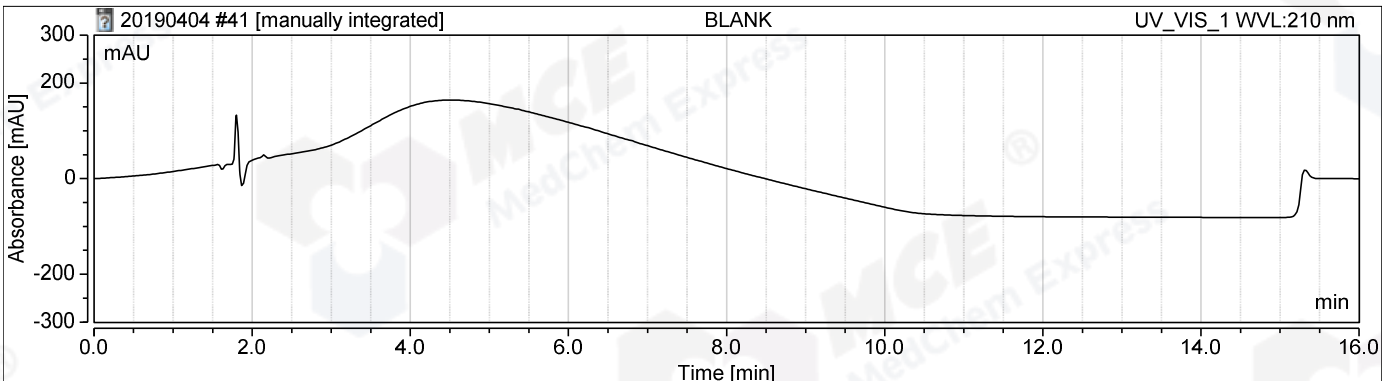


Chromatogram and Results

Injection Details

Injection Name: BLANK	Run Time (min): 16.00
Vial Number: RA3	Users: zqq
Injection Type: Unknown	Injection Volume: 5.00
Calibration Level:	Channel: UV_VIS_1
Instrument Method: 10-90A 214NM	Wavelength: 210
Processing Method: 3D Quantitative	Bandwidth: 4
Comment: BLANK A-RP-328	Dilution Factor: 1.0000
Injection Date/Time: 05/Apr/19 02:10	Sample Weight: 1.0000

Chromatogram

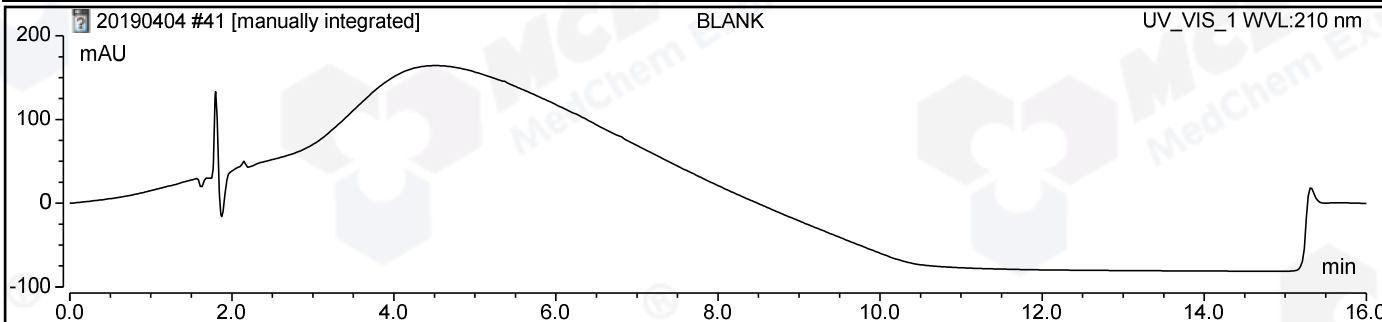

Integration Results



No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Resolution (EP)	Match	Asymmetry (EP)	Rel.Area %
Total:			0.000	0.000	0.00			0.00

Chromatogram and Results

Injection Details

Injection Name: CPK2019-404-11310	Run Time (min): 16.00
Vial Number: RE8	Users: zqq
Injection Type: Unknown	Injection Volume: 5.00
Calibration Level:	Channel: UV_VIS_1
Instrument Method: 10-90A 214NM	Wavelength: 210
Processing Method: 3D Quantitative	Bandwidth: 4
Comment: HY-B0217-20190401 A-RP-328	Dilution Factor: 1.0000
Injection Date/Time: 05/Apr/19 04:54	Sample Weight: 1.0000

Chromatogram

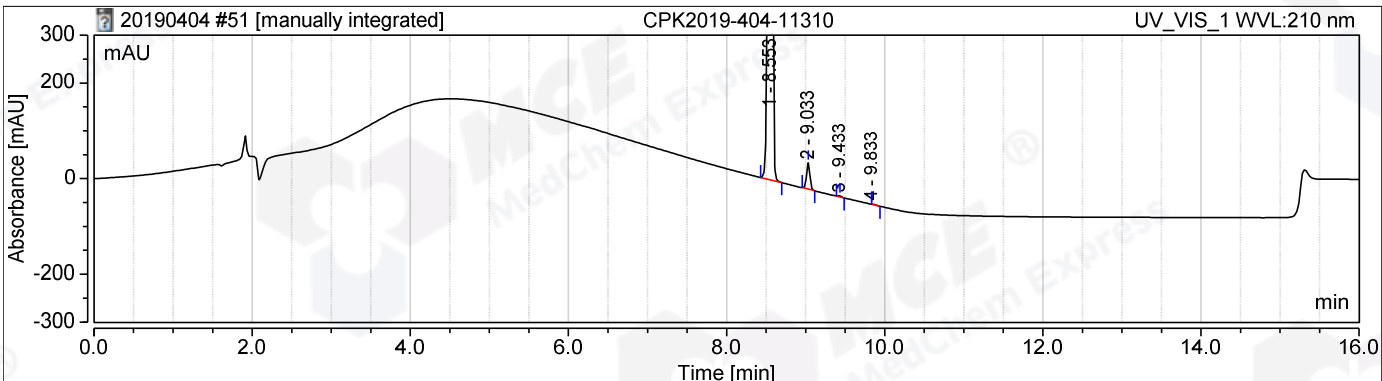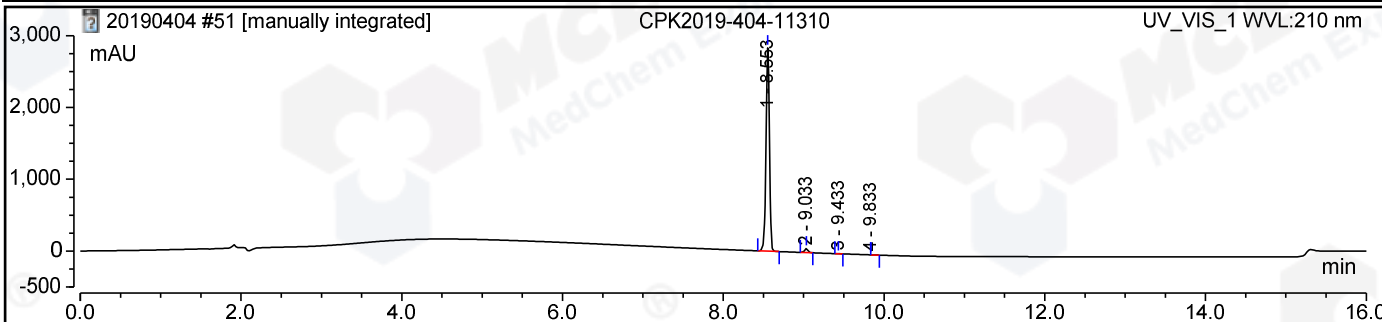

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Resolution (EP)	Match	Asymmetry (EP)	Rel.Area %
1		8.553	136.348	2835.687	6.51	963	0.93	98.03
2		9.033	2.579	55.122	5.61	1000	0.96	1.85
3		9.433	0.103	2.361	n.a.	956	1.12	0.07
4		9.833	0.061	0.000	n.a.	1000	n.a.	0.04
Total:			139.091	2893.170	12.11			3.01