



File ..1\DATA\2019\20190221\554\BIZ2019-220-WYQ1.D Tgt Mass (CHM):
Injection Date : 21 Feb 19 12:26 pm +0800 Seq. Line : 30
Sample Name : BIZ2019-220-WYQ1 Location : P2-D-06
Acq. Operator : LQ_1052 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2019\20190221\554\1-POS-3MIN-1.M
Analysis Method : D:\CHEM32\1\DATA\2019\20190221\554\1-POS-3MIN-1.M
Catalog No : HY-B0280 Batch#37671
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-314
Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

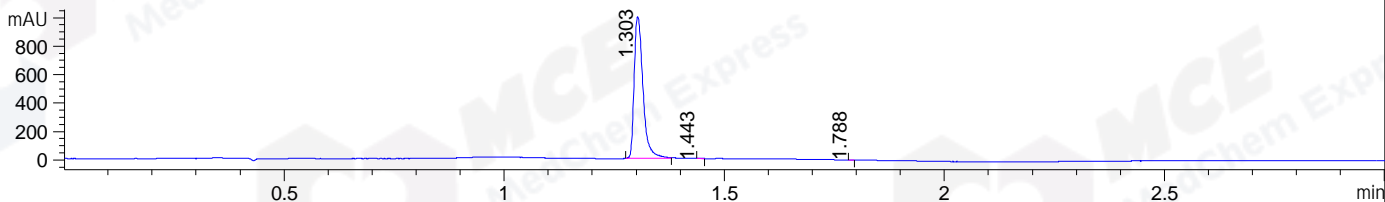


DAD1 C, Sig=254,4 Ref=off

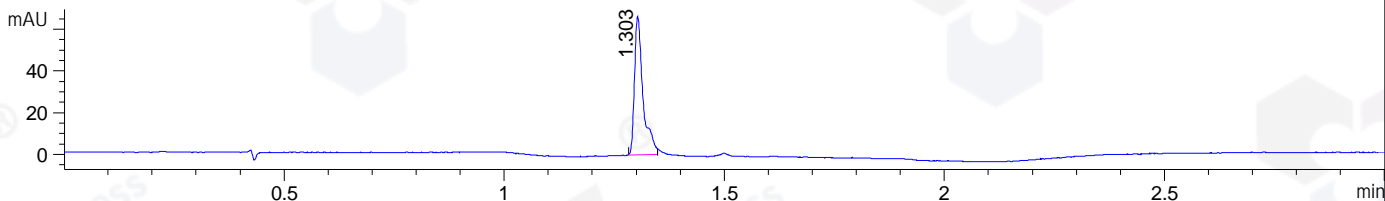

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

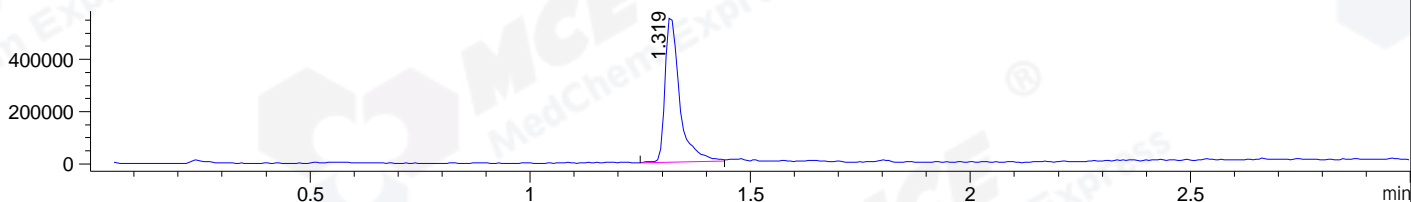

Ion 428.2, MSD1 428.2, Target Mass 427.2 +H Positive, EIC=427.9:428.9

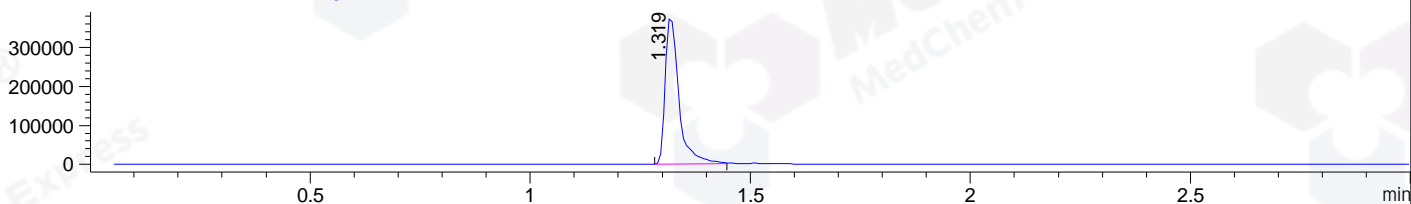

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.30	0.02	1392.36	997.73	99.91	428
1.44	0.01	0.96	1.40	0.07	428
1.79	0.01	0.26	0.60	0.02	327

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.30	0.02	89.58	66.40	100.00	428

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.32	0.03	1279807.88	565887.44	100.00	428

Ret. Time: 1.32

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

