



File ..DATA\2020\20201106\1146\CPK2020-N05-16018.D Tgt Mass (CHM):  
 Injection Date : 6 Nov 20 2:38 pm +0800 Seq. Line : 58  
 Sample Name : CPK2020-N05-16018 Location : P1-B-02  
 Acq. Operator : zyj\_1547 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2020\20201106\1146\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2020\20201106\1146\1-POS-3MIN.M  
 Catalog No : HY-B0327  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

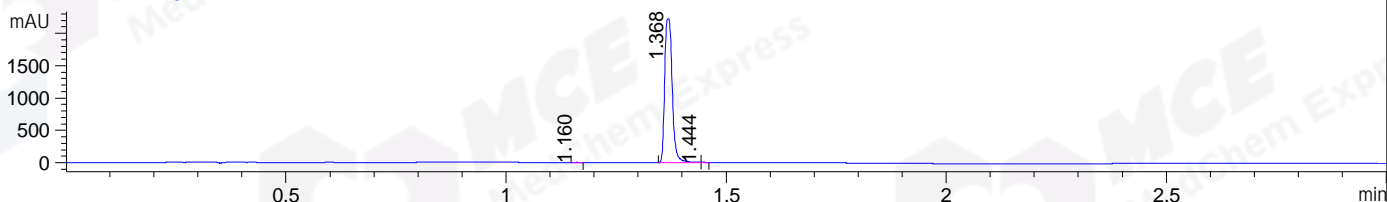


DAD1 C, Sig=254,4 Ref=off

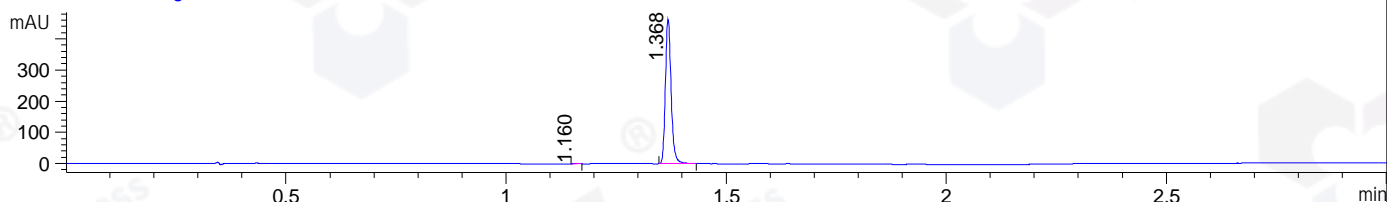

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

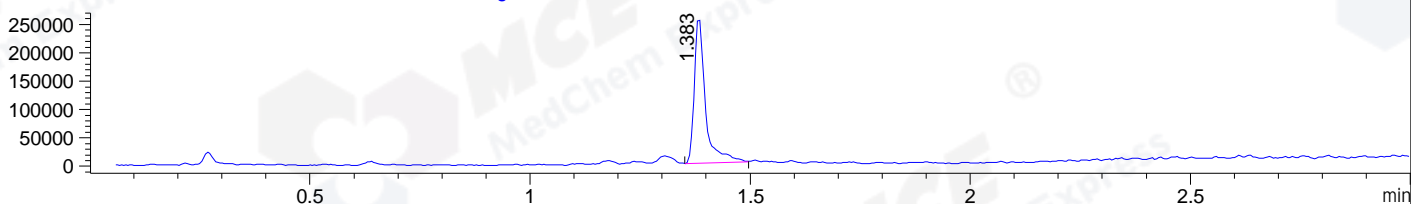

Ion 256, MSD1 256, Target Mass 255 +H Positive, EIC=255.7:256.7

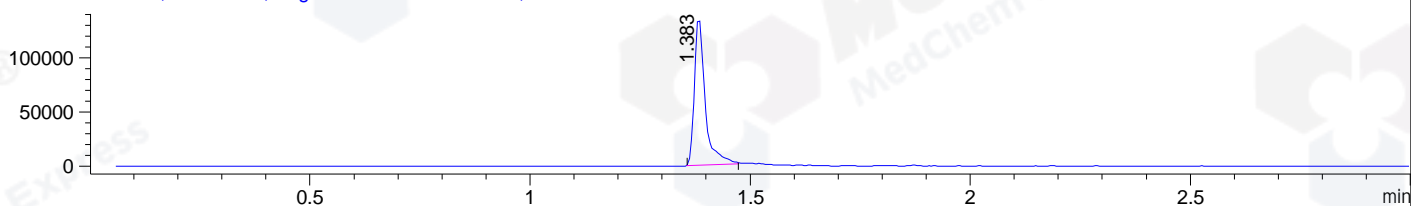

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.16	0.01	3.85	5.07	0.15	296
1.37	0.02	2628.38	2224.76	99.80	256
1.44	0.01	1.43	2.27	0.05	256

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.16	0.01	0.69	0.95	0.16	ND
1.37	0.02	418.25	464.69	99.84	256

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.38	0.03	449946.84	257577.16	100.00	256

Ret. Time: 1.38

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

