
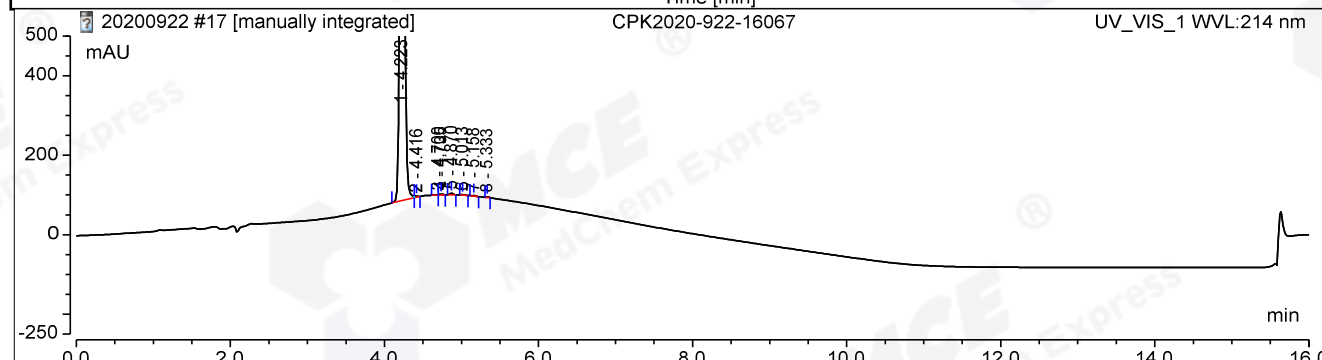


Chromatogram and Results

Injection Details			
Injection Name:	CPK2020-922-16067	Injection Volume:	2.00
Vial Number:	BC6	Channel:	UV_VIS_1
Injection Type:	Unknown	Wavelength:	214
Calibration Level:		Users:	jlw
Instrument Method:	10-90A,214NM	Dilution Factor:	1.0000
Processing Method:	New Processing Method	Sample Weight:	1.0000
Injection Date/Time:	22/Sep/20 18:49	Run Time (min):	16.00
Comment:	20200915 A-RP-536		
chrom://hy261/Themo/Instrument Data/202009/20200922.seq/756.smp/UV_VIS_1.channel/UV_VIS_1.chm			

Chromatogram

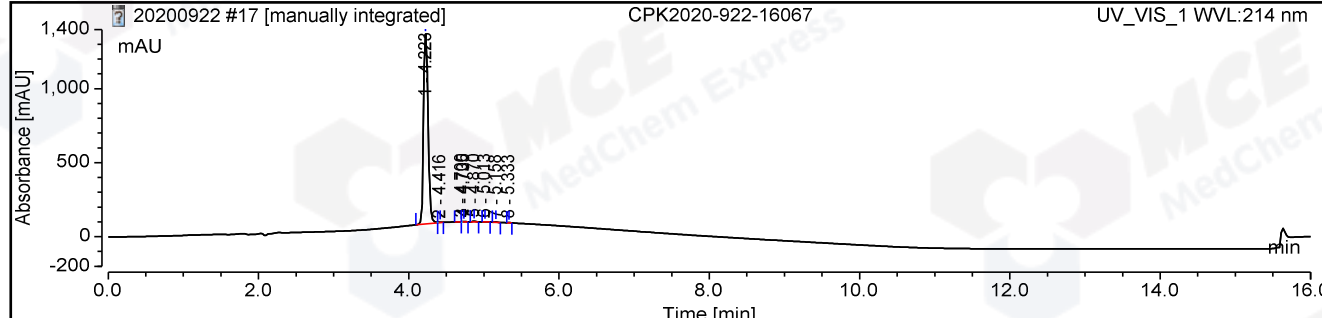

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Asymmetry (EP)	S/N	Rel.Area %
1		4.223	90.119	1282.550	1.24	790.2	99.26
2		4.416	0.155	2.676	n.a.	1.6	0.17
3		4.700	0.053	0.863	n.a.	0.5	0.06
4		4.735	0.100	2.024	n.a.	1.2	0.11
5		4.870	0.188	4.075	1.07	2.5	0.21
6		5.013	0.050	1.193	1.13	0.7	0.05
7		5.158	0.065	1.567	1.40	1.0	0.07
8		5.333	0.065	2.069	1.13	1.3	0.07
Total:			90.795	1297.015	5.97	799.10	