



File ..DATA\2021\20210310\1299\CPK2021-305-16381.D Tgt Mass (CHM):  
Injection Date : 10 Mar 21 9:24 pm +0800 Seq. Line : 154  
Sample Name : CPK2021-305-16381 Location : P1-F-02  
Acq. Operator : yrz\_1364 Inj : 1  
Spec. Reported : MS Integration Inj Volume : 1 ul  
Acq. Method : D:\Chem32\1\data\2021\20210310\1299\1-POS-3MIN.M  
Analysis Method : D:\CHEM32\1\DATA\2021\20210310\1299\1-POS-3MIN.M  
CAS NO. : 181183-52-8  
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
Gradient: 5% to 95%B within 1.3 min  
Flow Rate :1.8ml/min  
Column :SunFire C18, 4.6\*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

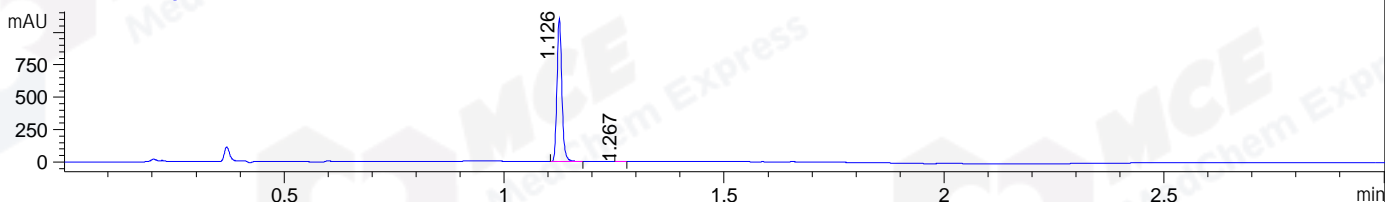


DAD1 C, Sig=254,4 Ref=off

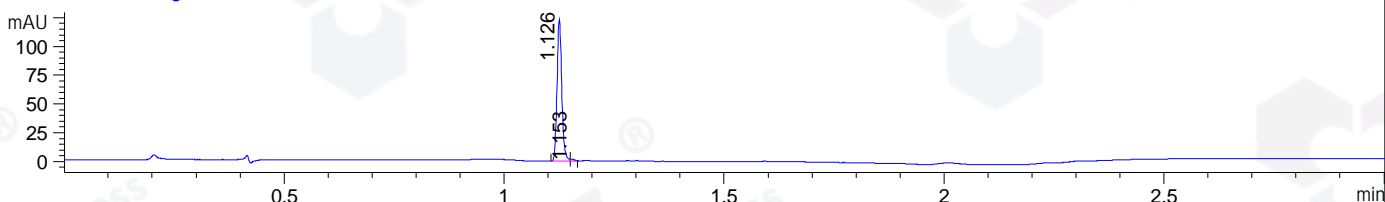

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

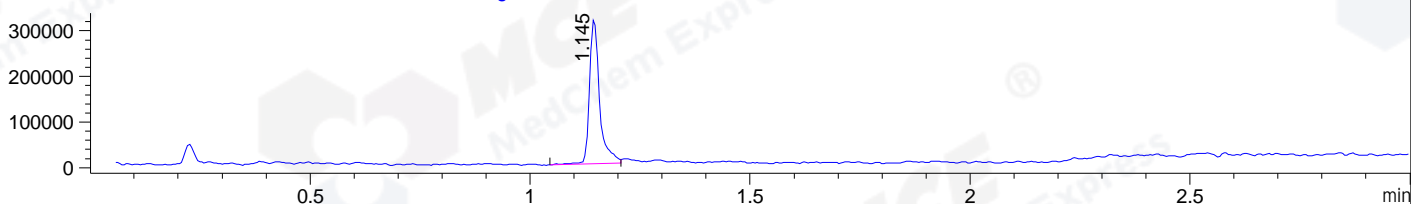

Ion 336, MSD1 336, Target Mass 335 +H Positive, EIC=335.7:336.7

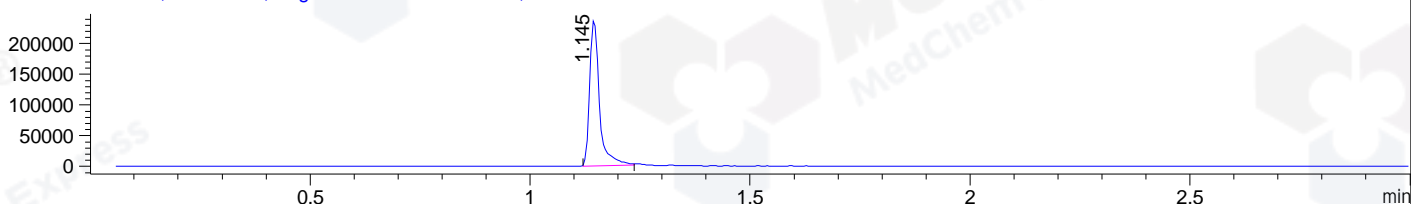

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.13	0.01	858.38	1107.44	99.91	336
1.27	0.01	0.81	1.16	0.09	336

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.13	0.01	92.69	123.68	99.06	336
1.15	0.01	0.88	1.39	0.94	336

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.14	0.02	508293.72	31996.28	100.00	336

Ret. Time: 1.14

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

