



File ..TA\2020\20201127\1168 1\CPK2020-N27-16841.D Tgt Mass (CHM):
 Injection Date : 27 Nov 20 11:38 pm +0800 Seq. Line : 160
 Sample Name : CPK2020-N27-16841 Location : P1-D-01
 Acq. Operator : zyj_1547 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20201127\1168 1\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20201127\1168 1\1-POS-3MIN.M
 CAS NO. : 74711-43-6
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

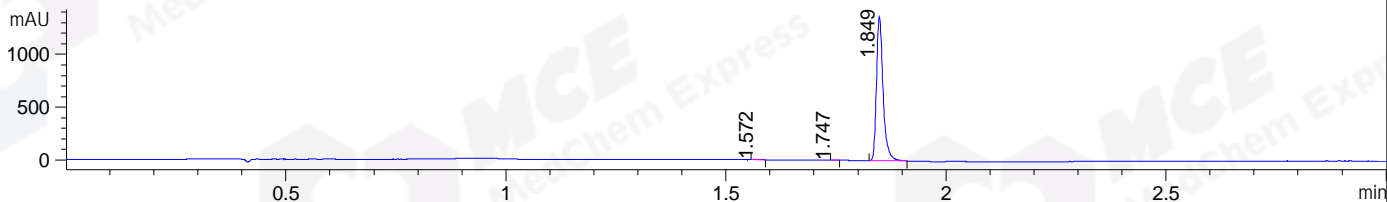


DAD1 C, Sig=254,4 Ref=off

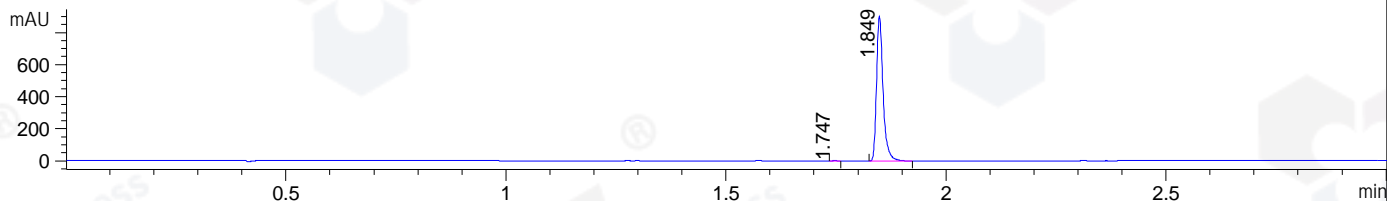

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

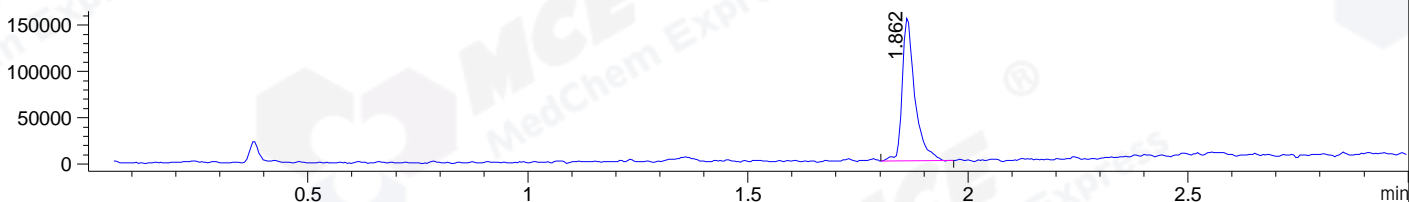

Ion 299, MSD1 299, Target Mass 298 +H Positive, EIC=298.7:299.7

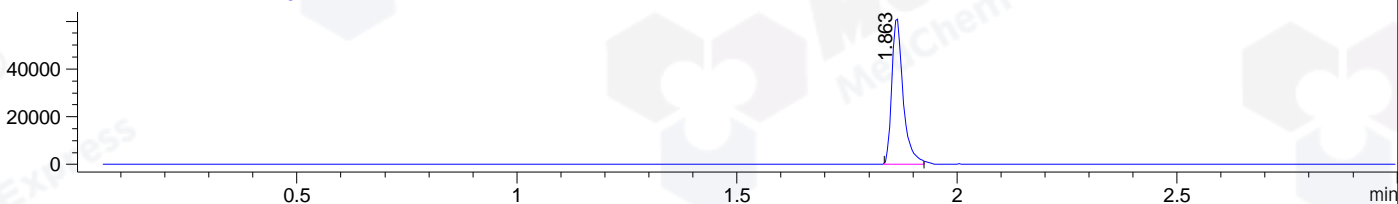

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.57	0.02	3.64	3.69	0.25	ND
1.75	0.01	1.34	2.07	0.09	ND
1.85	0.02	1423.78	1367.83	99.65	299

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.75	0.01	1.15	1.47	0.12	ND
1.85	0.02	936.04	904.86	99.88	299

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.86	0.03	311433.09	155425.59	100.00	299

Ret. Time: 1.86

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

