



File ..DATA\2020\20200818\1075\CPK2020-814-26966.D Tgt Mass (CHM):  
 Injection Date : 18 Aug 20 3:57 pm +0800 Seq. Line : 12  
 Sample Name : CPK2020-814-26966 Location : P1-C-02  
 Acq. Operator : zyj\_1547 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2020\20200818\1075\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2020\20200818\1075\1-POS-3MIN.M  
 Catalog No : HY-B0808  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-607  
 Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

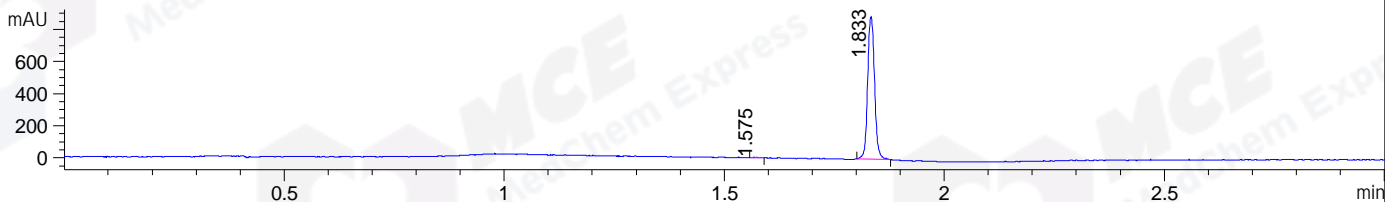


DAD1 C, Sig=254,4 Ref=off

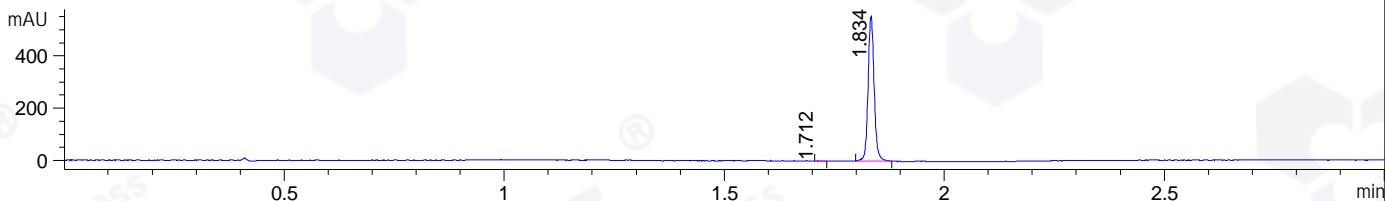

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

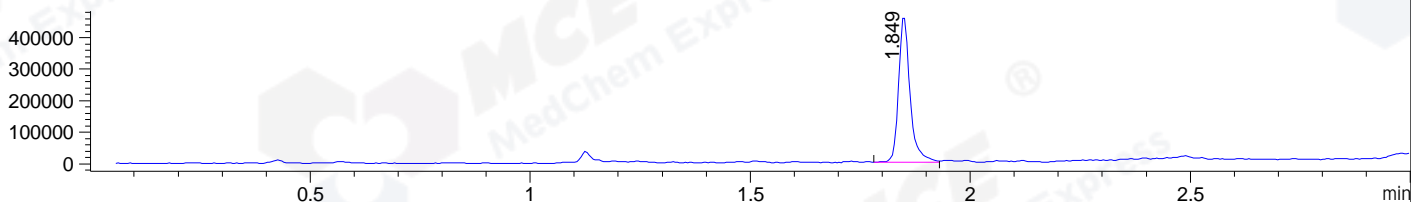

Ion 294, MSD1 294, Target Mass 293 +H Positive, EIC=293.7:294.7

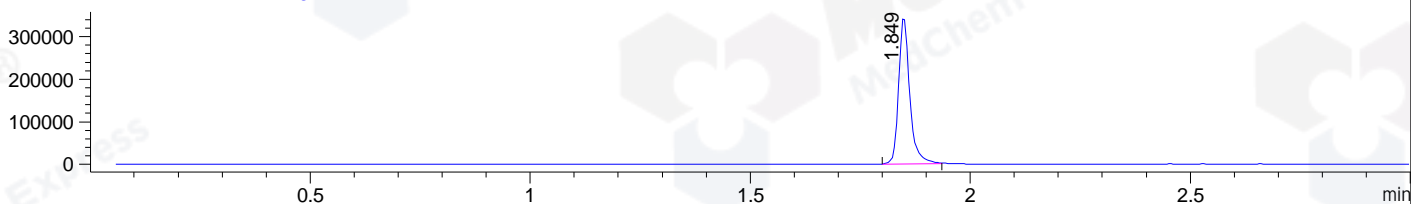

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.57	0.02	3.80	3.09	0.39	ND
1.83	0.02	970.03	889.72	99.61	294

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.71	0.01	1.24	1.52	0.24	ND
1.83	0.02	526.36	553.45	99.76	294

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.85	0.03	844437.44	467105.97	100.00	294

Ret. Time: 1.85

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

