
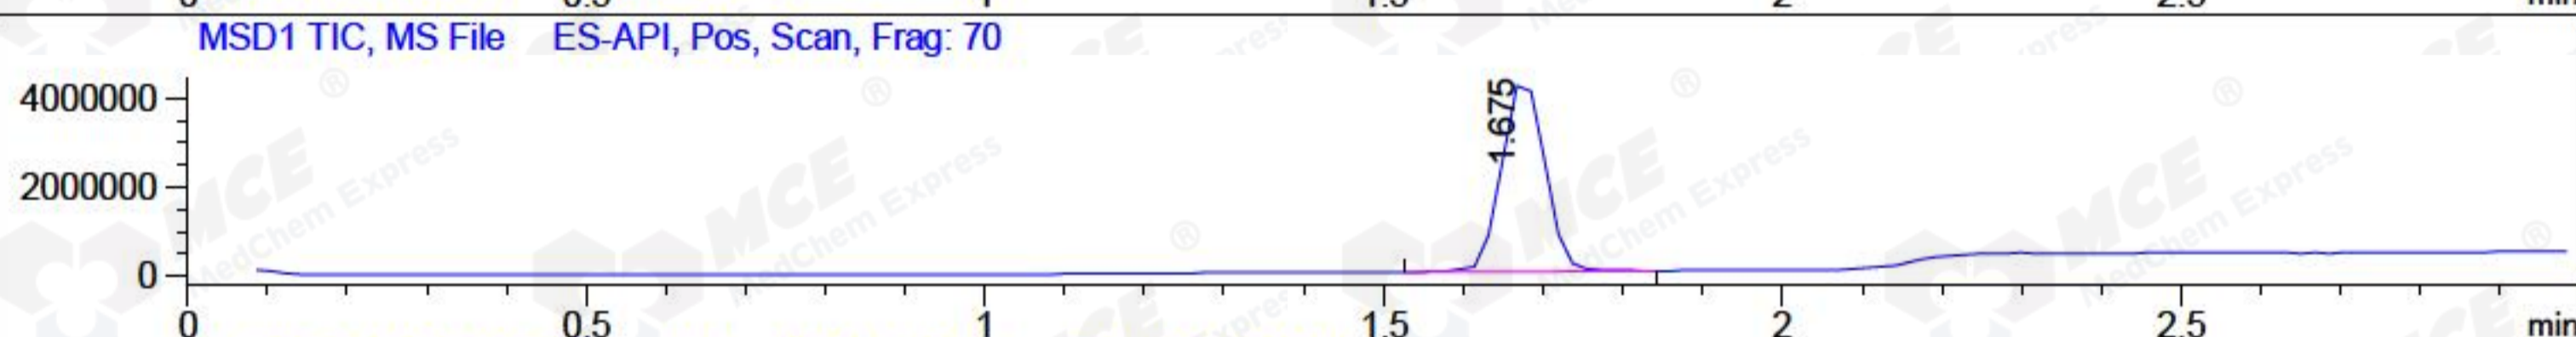
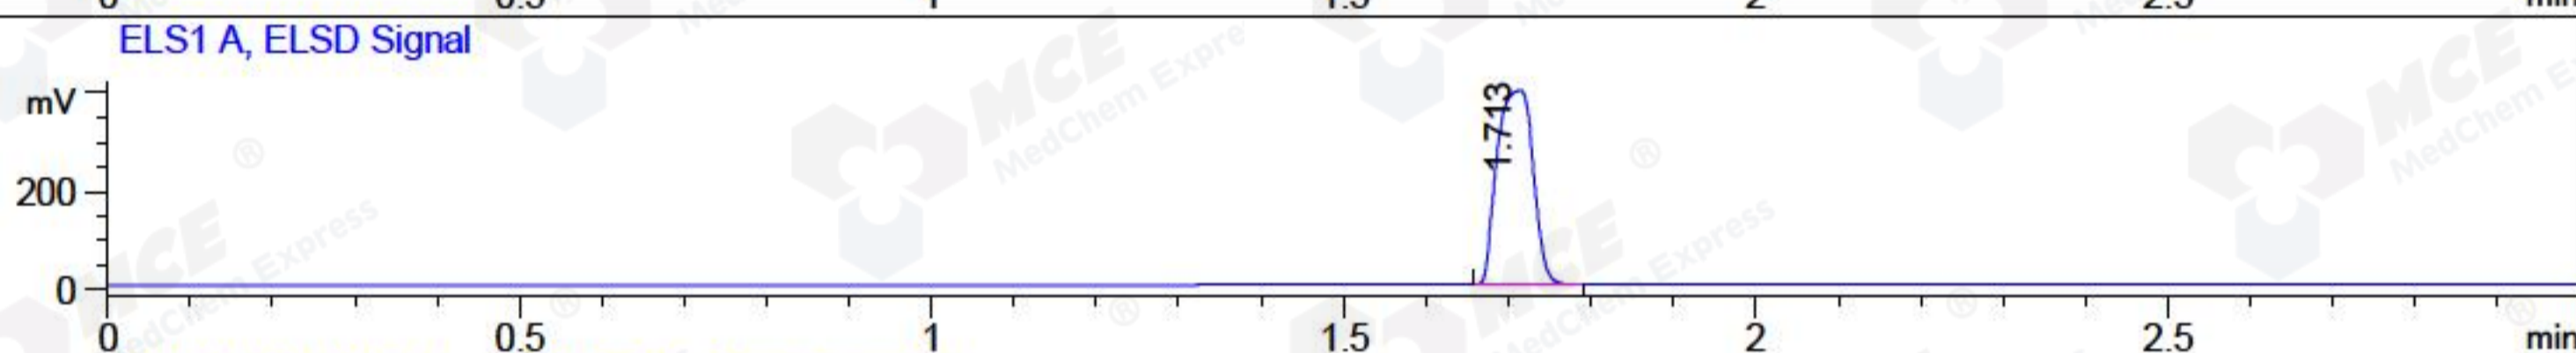
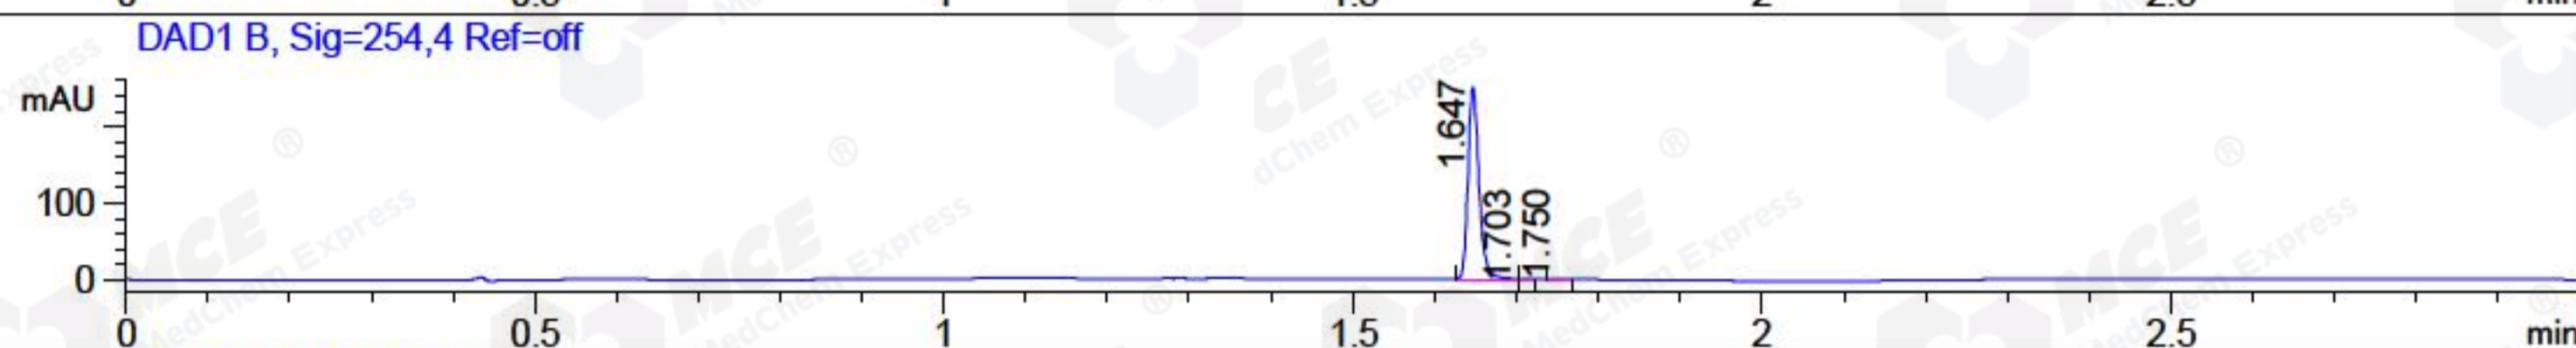


File ..3\Data\20171107\20171107\BIZ2017-N07-WYQ1.D Tgt Mass (CHM):  
 Injection Date : 7 Nov 17 12:11 pm +0800 Seq. Line : 45  
 Sample Name : BIZ2017-N07-WYQ1 Location : P1-D-06  
 Acq. Operator : SYSTEM Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\LCMS03\Data\20171107\20171107\1-POS-3MIN.M  
 Analysis Method : D:\LCMS03\Data\20171107\20171107\1-POS-3MIN.M  
 Catalog No : HY-B1330 Batch#27102  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-186  
 Oven Temperature : 45C

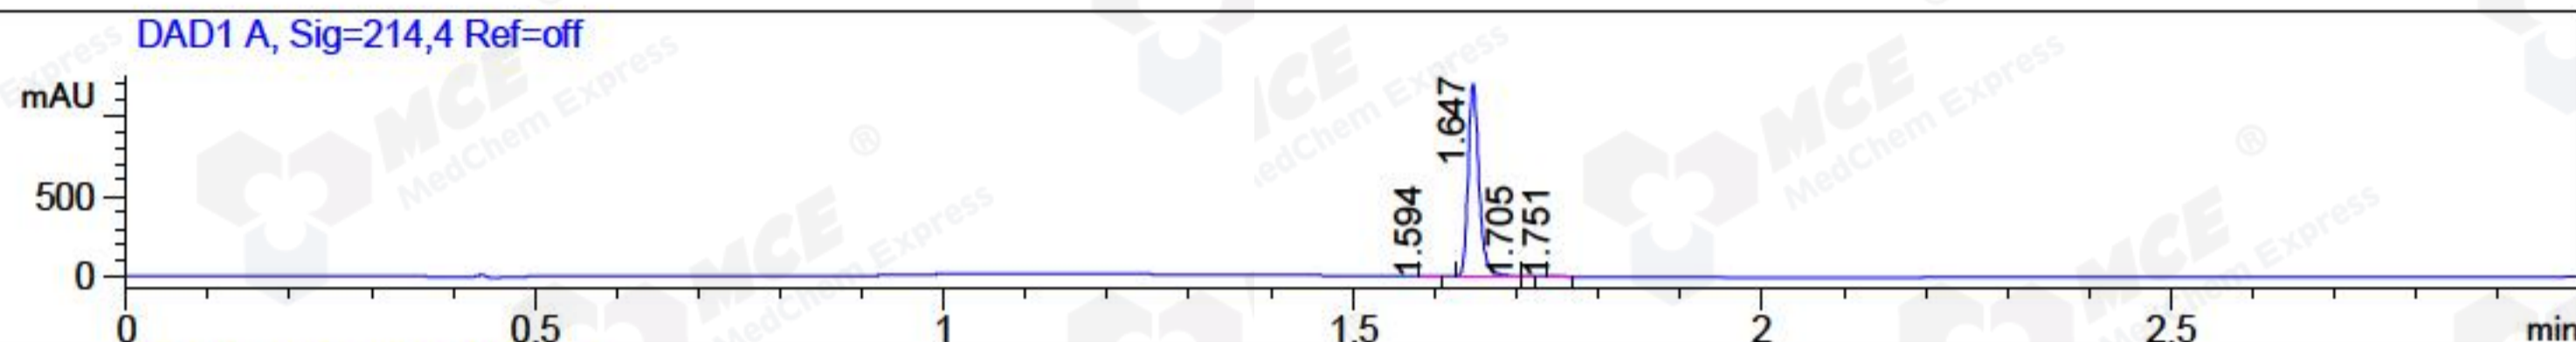

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.59	0.01	0.73	0.90	0.07	144
1.65	0.02	1094.16	1189.73	99.74	335
1.70	0.01	0.66	1.33	0.06	335
1.75	0.01	1.51	1.77	0.14	335

Integration Results for DAD1 B, Sig=254,4 Ref=off


RetTim	Width	Area	Height	Area%	MS (+)
1.65	0.02	231.44	248.91	99.69	335
1.70	0.01	0.15	0.28	0.06	335
1.75	0.01	0.58	0.66	0.25	335

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.67	0.06	16149030.00	4351042.00	100.00	335

Ret. Time: 1.67

<<<< POSITIVE SPECTRA >>>>

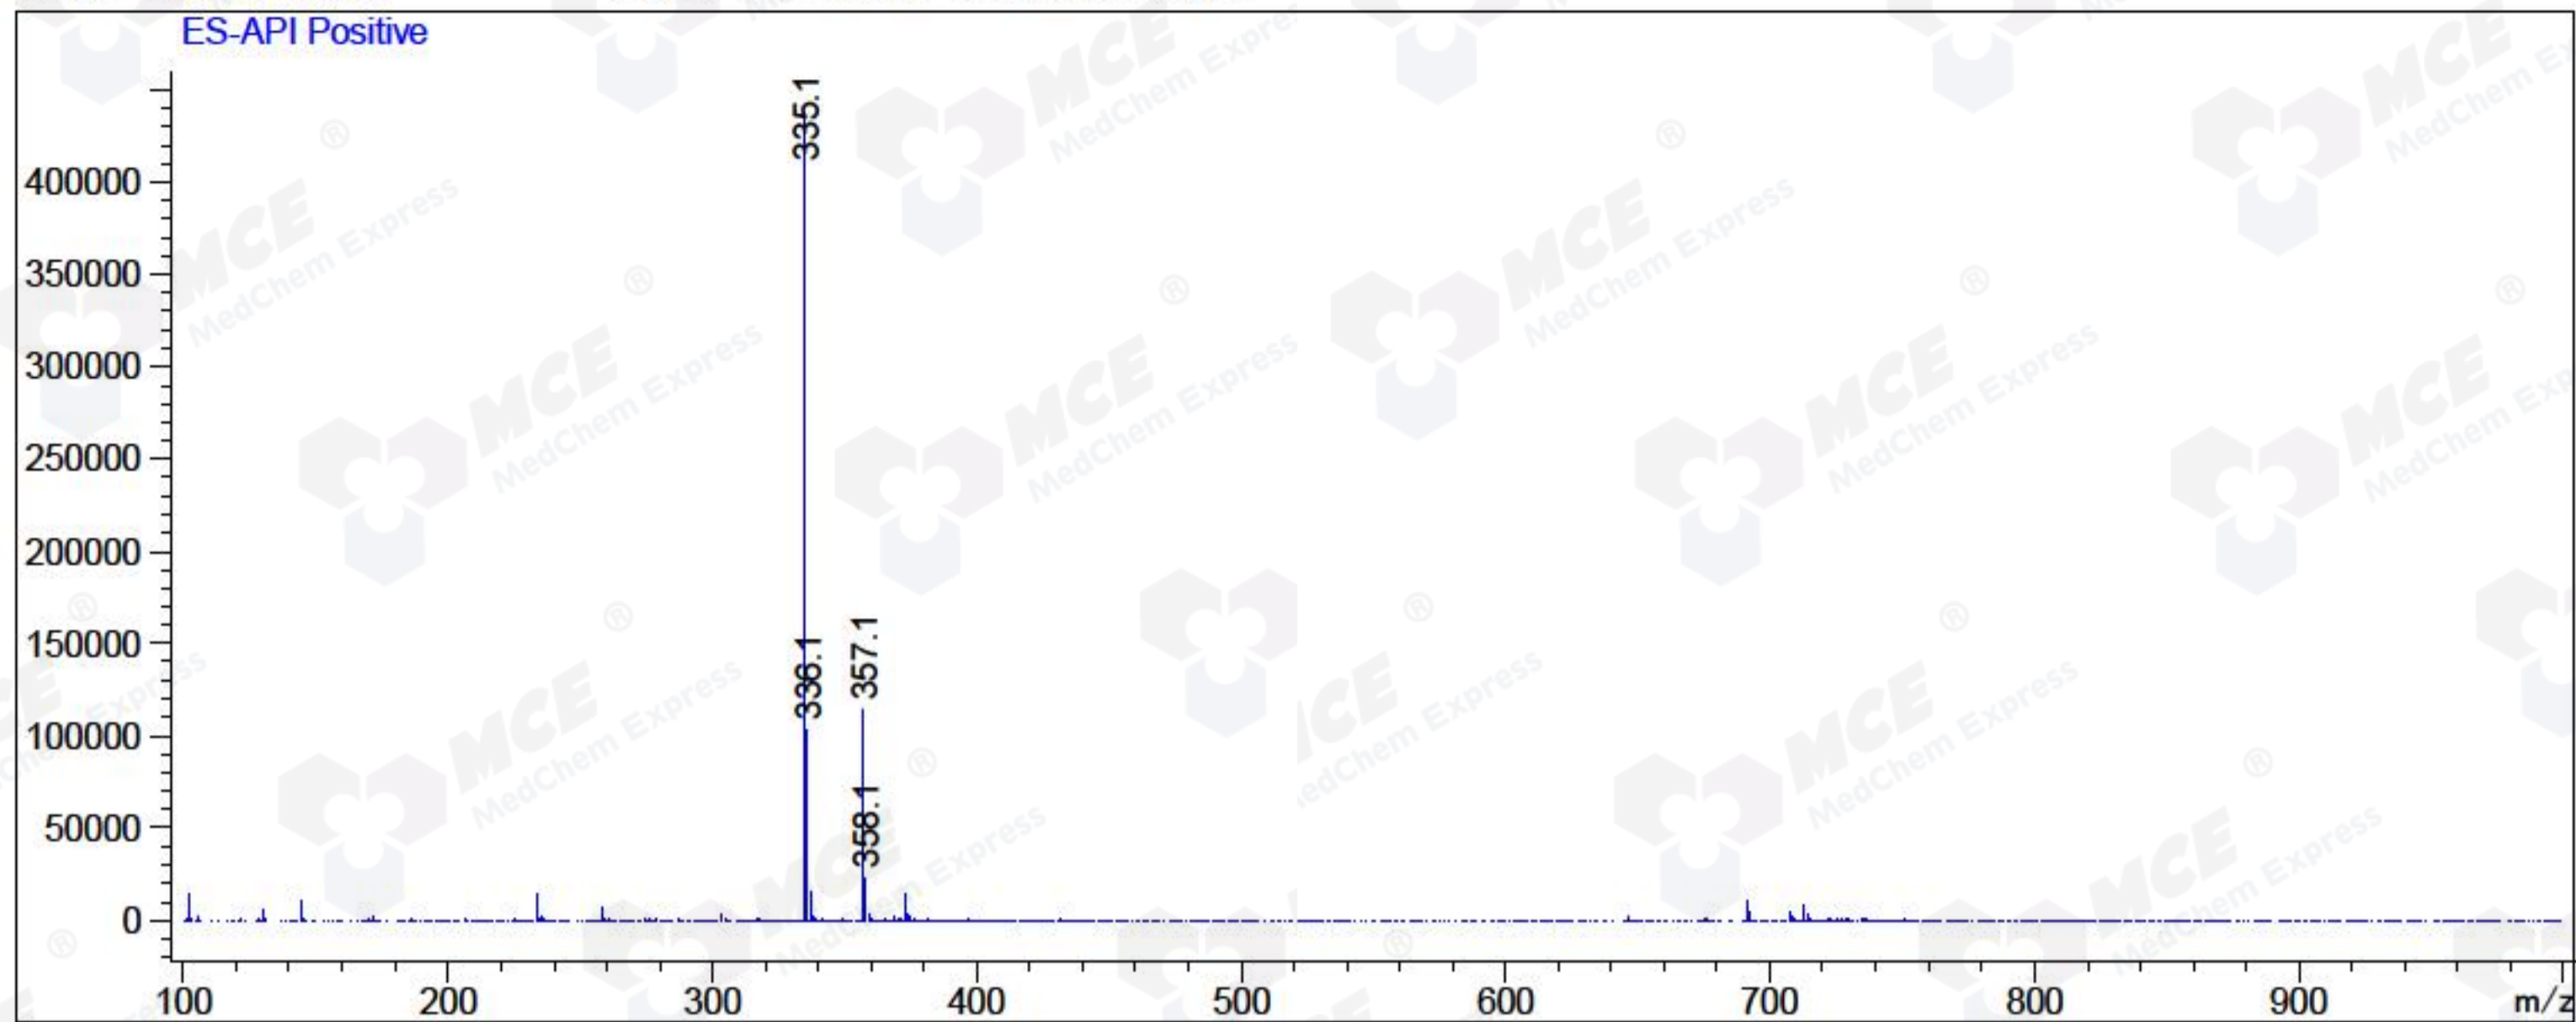

\*\*\* End of Report \*\*\*