
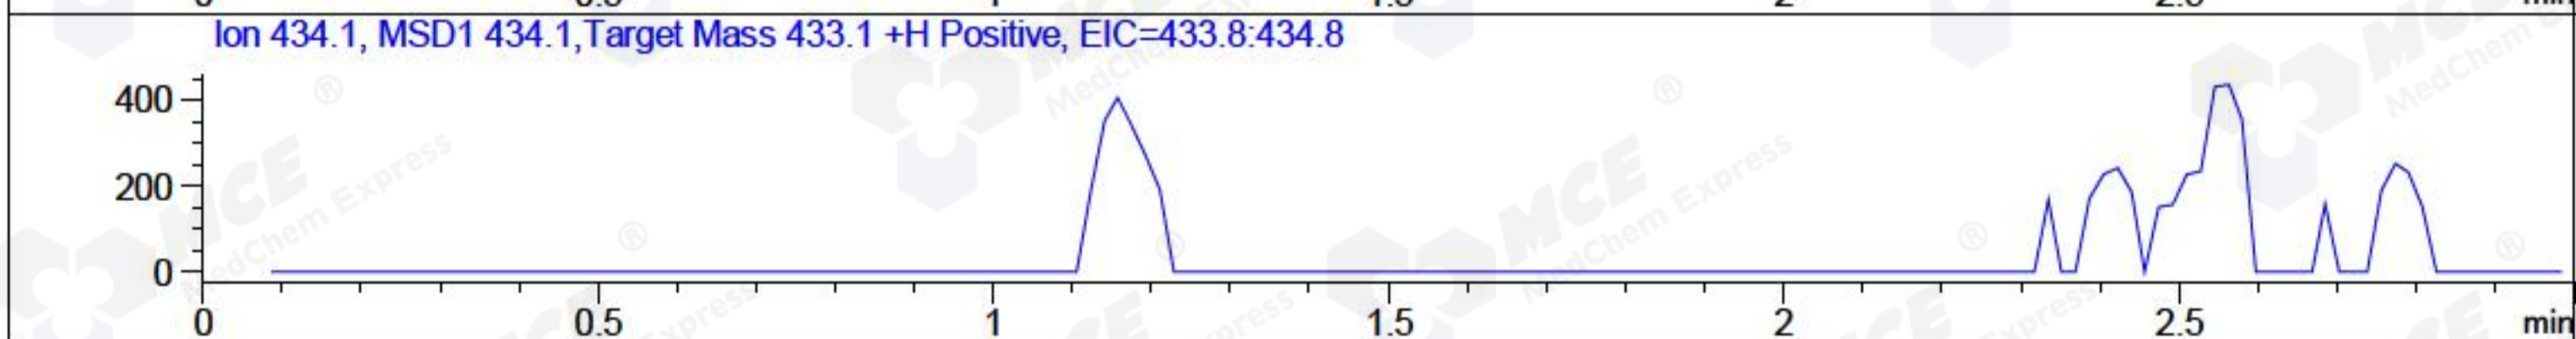
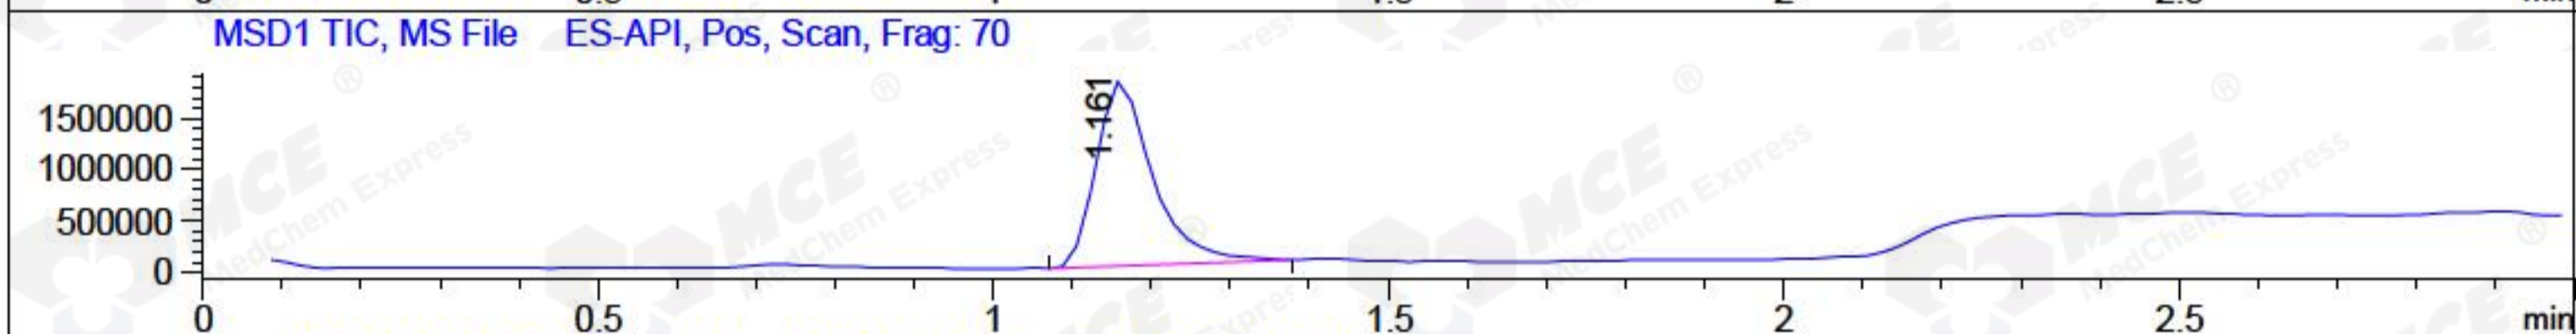
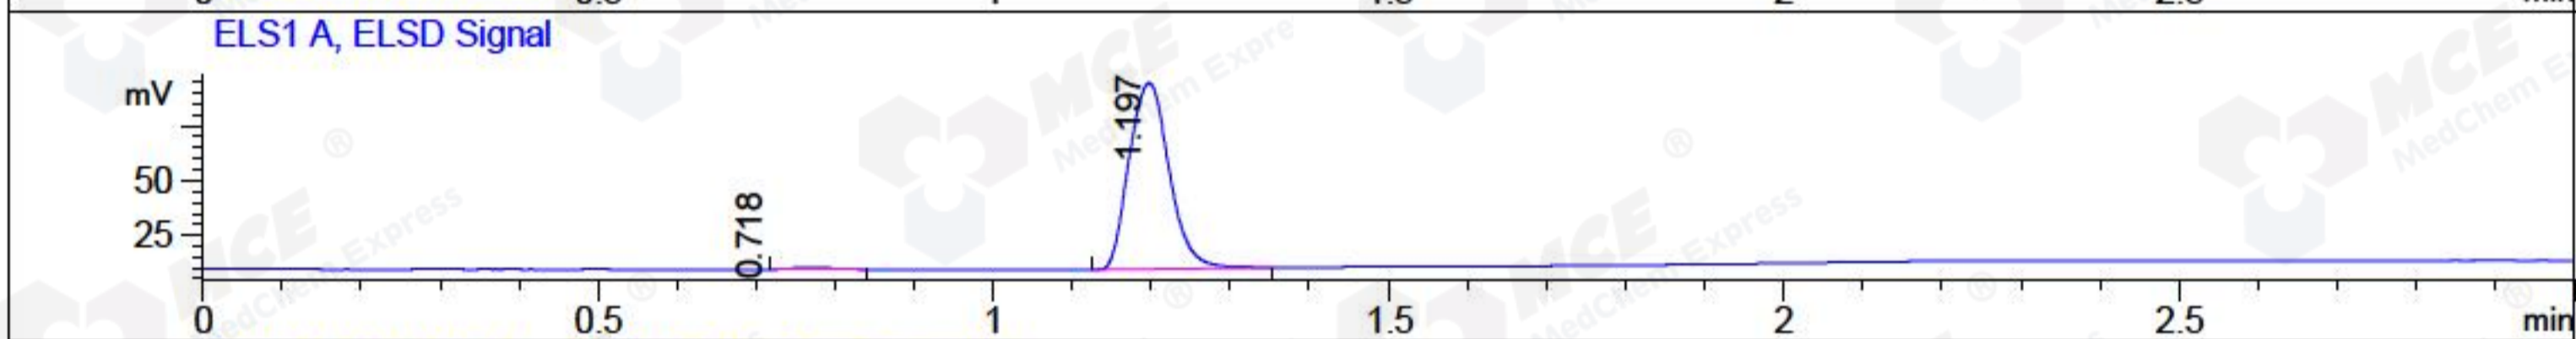
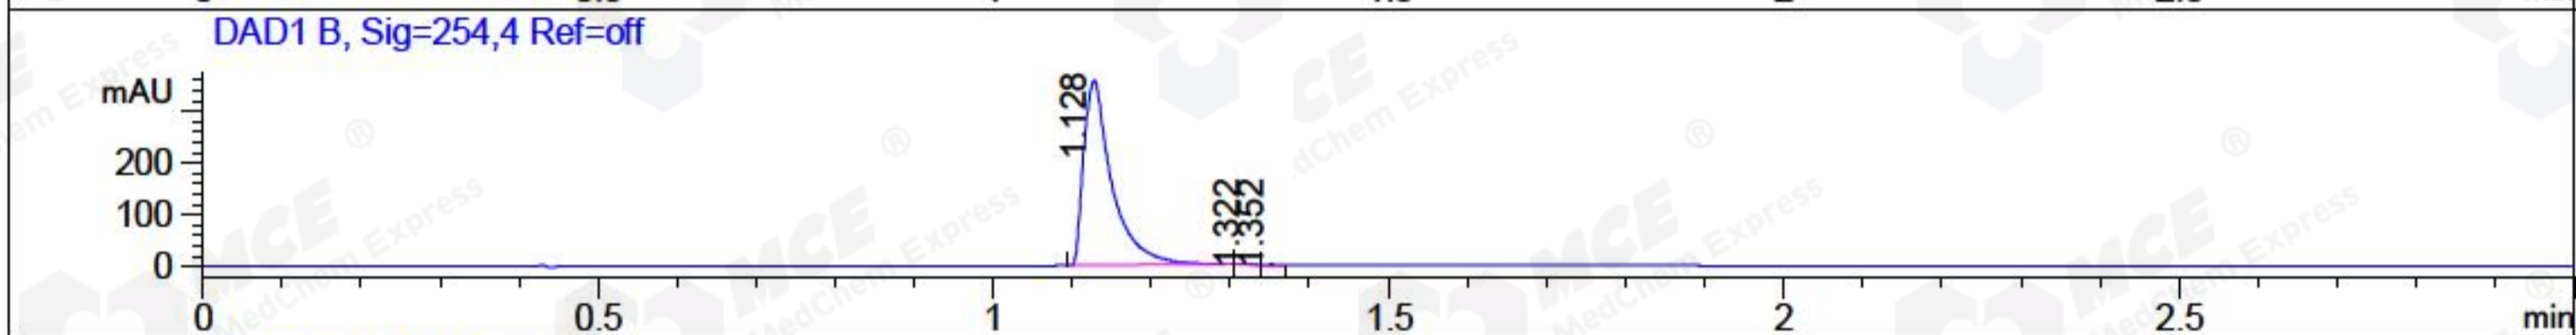


File ..ta\20171228\20171228-1\BIZ2017-D27-WYQ2-1.D Tgt Mass (CHM):
 Injection Date : 28 Dec 17 5:04 pm +0800 Seq. Line : 77
 Sample Name : BIZ2017-D27-WYQ2-1 Location : P2-A-01
 Acq. Operator : SYSTEM Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\LCMS03\Data\20171228\20171228-1\1-POS-3MIN.M
 Analysis Method : D:\LCMS03\Data\20171228\20171228-1\1-POS-3MIN.M
 Catalog No : HY-B1370 Batch#27976
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate : 1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-186
 Oven Temperature : 45C

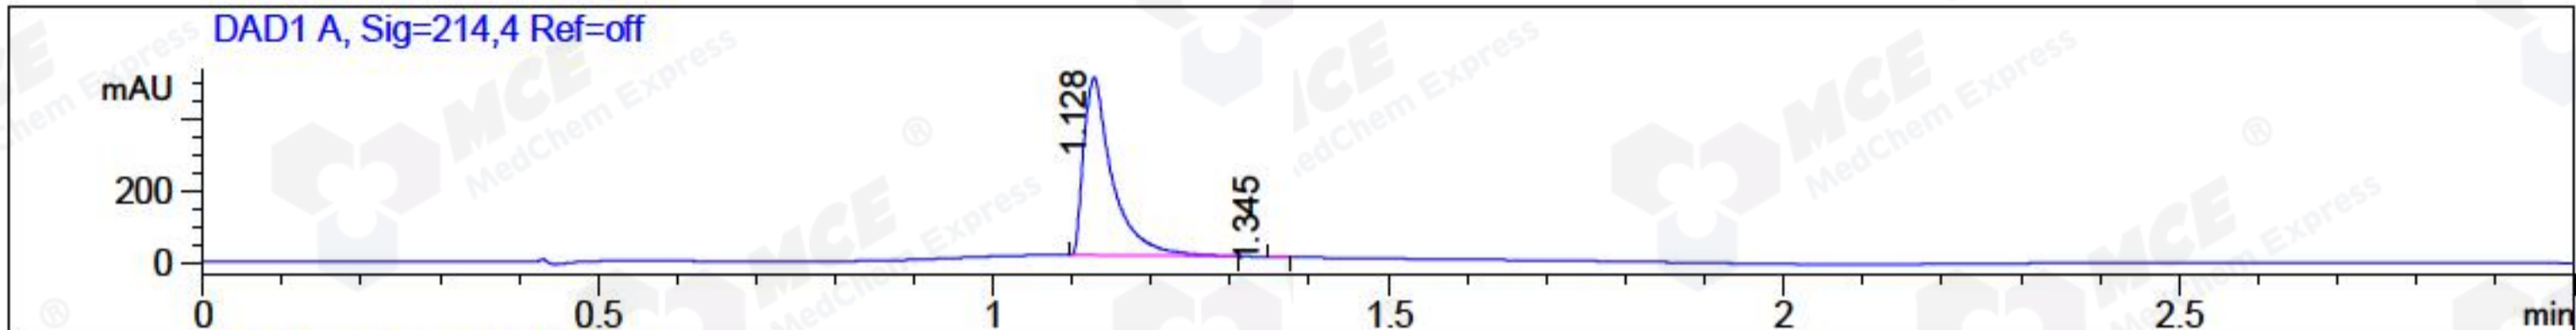

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.13	0.04	1253.29	496.75	99.99	336
1.35	0.01	0.13	-0.35	0.01	336

Integration Results for DAD1 B, Sig=254,4 Ref=off


RetTim	Width	Area	Height	Area%	MS (+)
1.13	0.04	894.70	356.21	99.92	336
1.32	0.02	0.48	0.49	0.05	336
1.35	0.02	0.26	0.26	0.03	336

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.16	0.07	8924700.00	1794543.38	100.00	336

Ret. Time: 1.16

<<<< POSITIVE SPECTRA >>>>

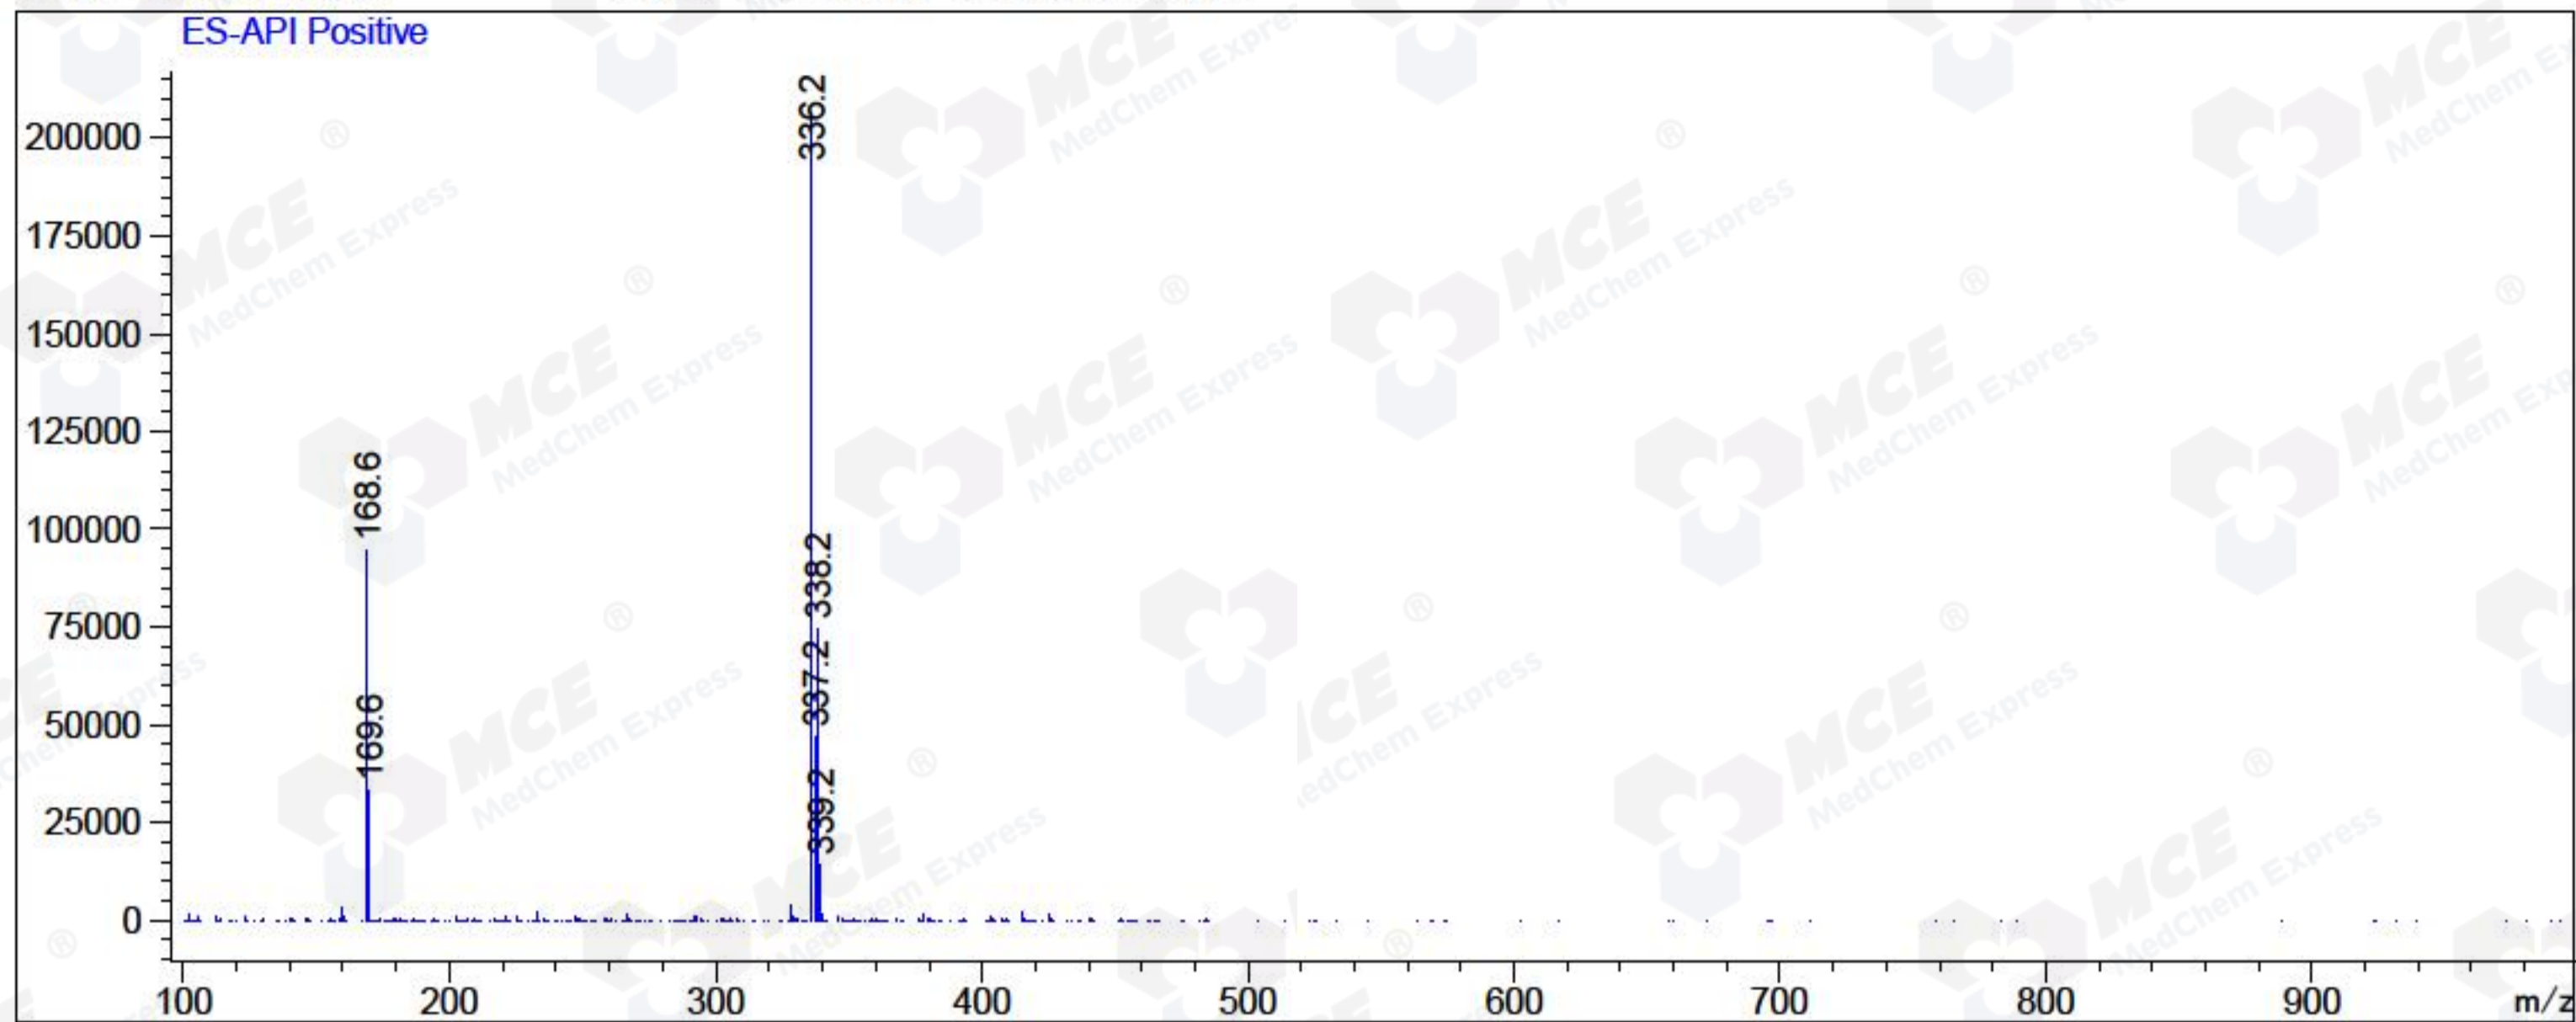

*** End of Report ***