



File ..DATA\2020\20200628\1018\CPK2020-623-27242.D Tgt Mass (CHM):
 Injection Date : 28 Jun 20 1:39 pm +0800 Seq. Line : 59
 Sample Name : CPK2020-623-27242 Location : P1-D-03
 Acq. Operator : ZJ_1432 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20200628\1018\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200628\1018\1-POS-3MIN.M
 Catalog No : HY-B1542A
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-607
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

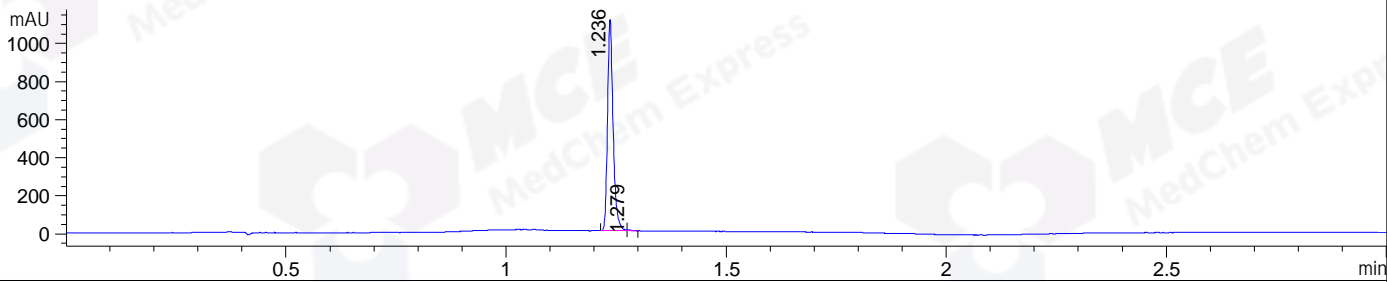

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

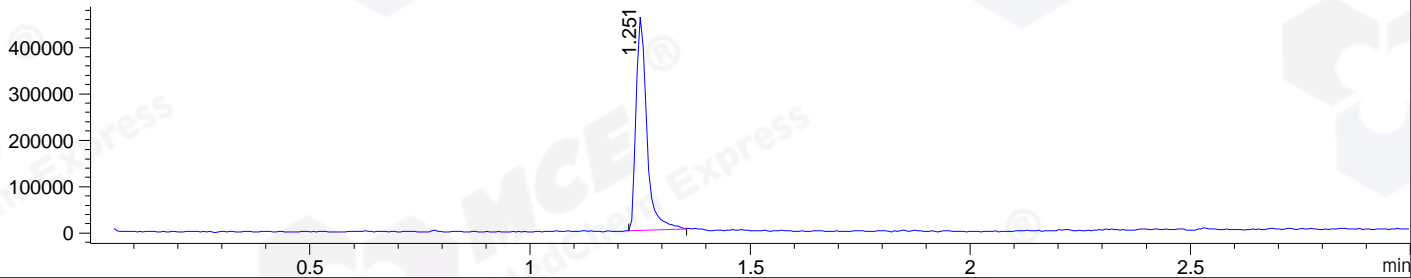

Ion 328, MSD1 328, Target Mass 327 +H Positive, EIC=327.7:328.7

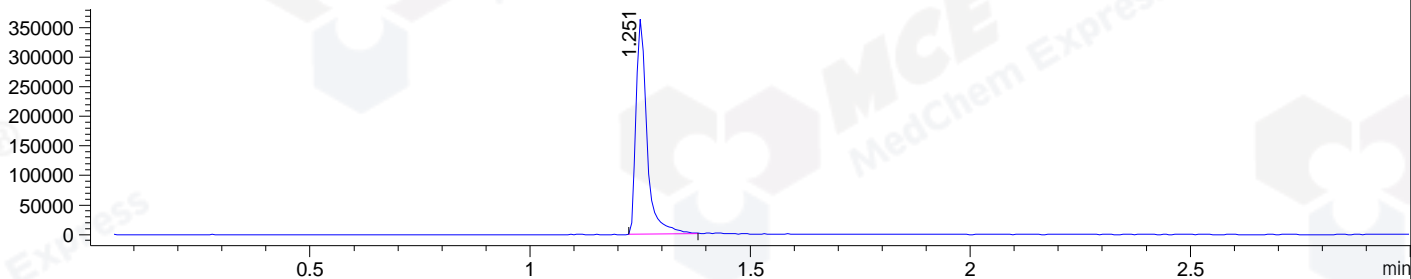

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.24	0.01	978.56	1110.40	99.69	328
1.28	0.01	3.07	3.73	0.31	328

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.25	0.03	782848.13	461319.81	100.00	328

Ret. Time: 1.25

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

