



File ..\DATA\2019\20190215\543\BIZ2019-215-WYQ25.D Tgt Mass (CHM):  
 Injection Date : 15 Feb 19 4:58 pm +0800 Seq. Line : 15  
 Sample Name : BIZ2019-215-WYQ25 Location : P2-C-03  
 Acq. Operator : LQ\_1052 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2019\20190215\543\1-POS-3MIN-1.M  
 Analysis Method : D:\CHEM32\1\DATA\2019\20190215\543\1-POS-3MIN-1.M  
 Catalog No : HY-B1839 Batch#38349  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-314  
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

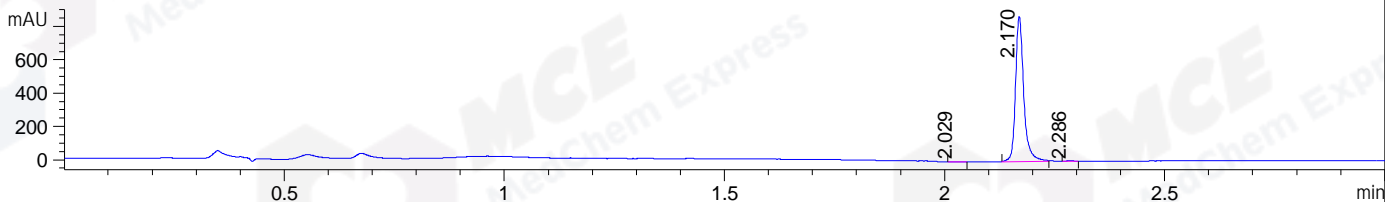


DAD1 C, Sig=254,4 Ref=off

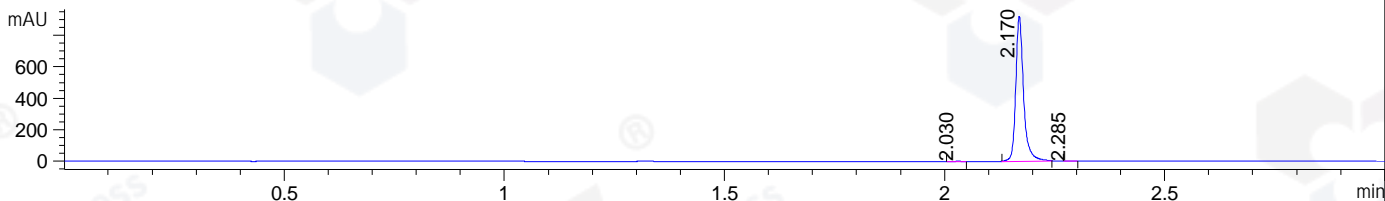

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

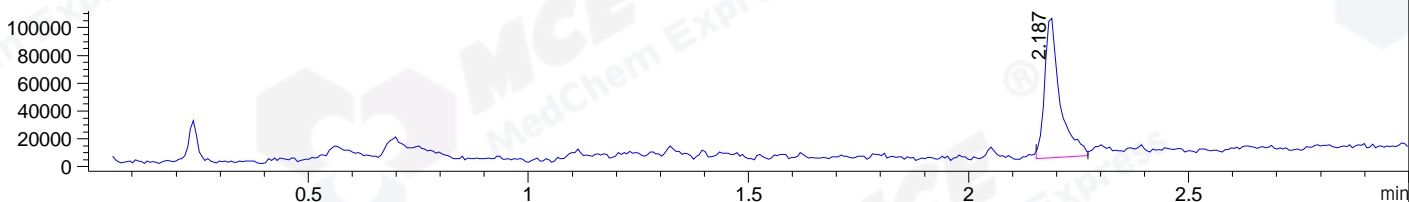

Ion 464.9, MSD1 464.9, Target Mass 463.9 +H Positive, EIC=464.6:465.6

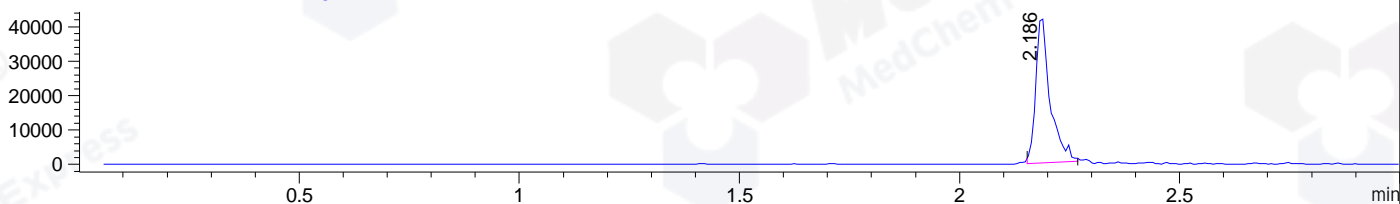

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
2.03	0.02	2.16	1.48	0.19	142
2.17	0.02	1137.80	871.59	99.54	465
2.29	0.02	3.07	2.94	0.27	142

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
2.03	0.02	3.48	2.60	0.30	142
2.17	0.02	1149.61	922.24	99.51	465
2.29	0.02	2.13	2.09	0.18	142

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
2.19	0.03	243149.31	102716.88	100.00	465

Ret. Time: 2.19

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

