



File ..\DATA\2020\20200923\1115\BIZ2020-922-SCH5.D Tgt Mass (CHM):
 Injection Date : 23 Sep 20 7:14 pm +0800 Seq. Line : 112
 Sample Name : BIZ2020-922-SCH5 Location : P1-A-04
 Acq. Operator : zyj_1547 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20200923\1115\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200923\1115\1-POS-3MIN.M
 CAS NO. : 57966-95-7
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-624


DAD1 B, Sig=214,4 Ref=off

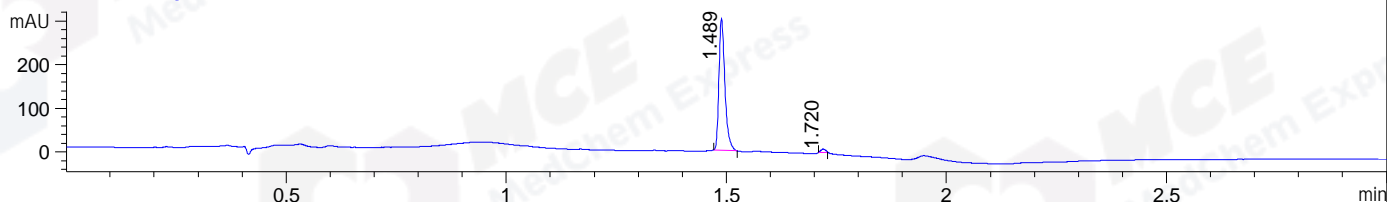


DAD1 C, Sig=254,4 Ref=off

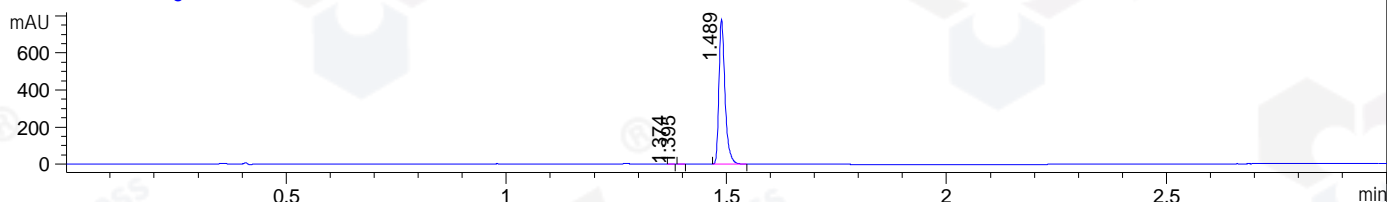

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

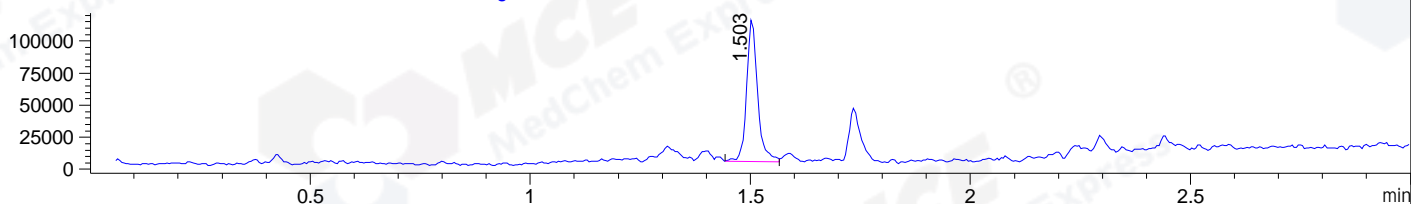

Ion 199, MSD1 199, Target Mass 198 +H Positive, EIC=198.7:199.7

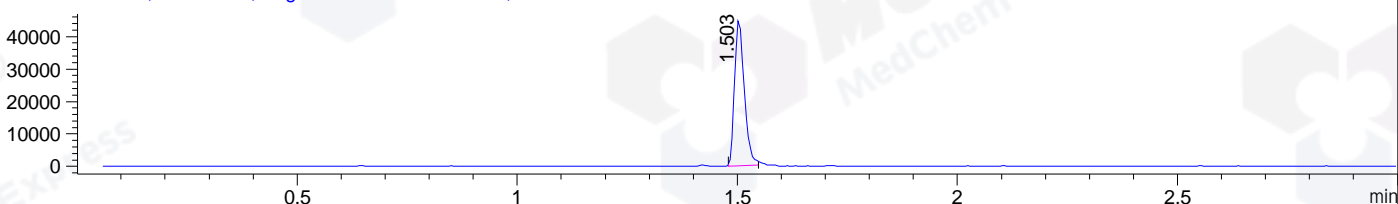

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.49	0.02	283.51	302.66	98.05	199
1.72	0.01	5.65	7.46	1.95	279

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.37	0.01	0.39	0.61	0.05	ND
1.40	0.01	0.34	0.55	0.05	978
1.49	0.02	747.57	784.12	99.90	199

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.50	0.03	189451.92	110861.35	100.00	199

Ret. Time: 1.50

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

