

File ..DATA\2020\20200311\867\CPK2020-309-26075-.D Tgt Mass (CHM):

Injection Date : 11 Mar 20 11:45 pm +0800 Seq. Line : 126

Sample Name : CPK2020-309-26075 Location : P1-B-08

Acq. Operator : ZJ\_1432 Inj : 1

Spec. Reported : MS Integration Inj Volume : 5 ul

Acq. Method : D:\Chem32\1\data\2020\20200311\867\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2020\20200311\867\1-POS-3MIN.M

Catalog No : HY-B2174 Batch#26075

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6\*50mm,3.5um A-RP-433

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

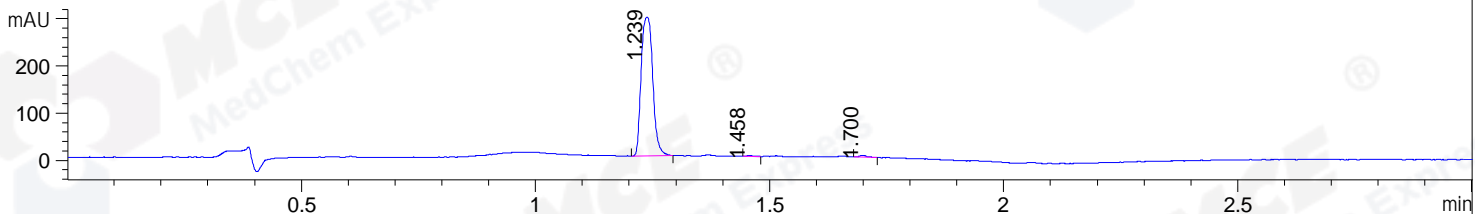


DAD1 C, Sig=254,4 Ref=off

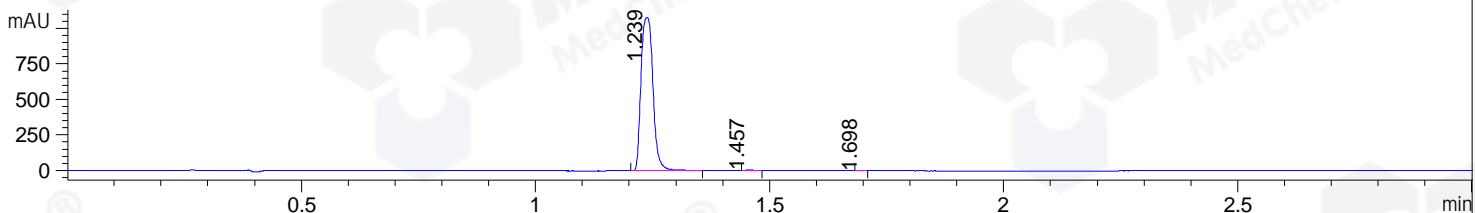

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

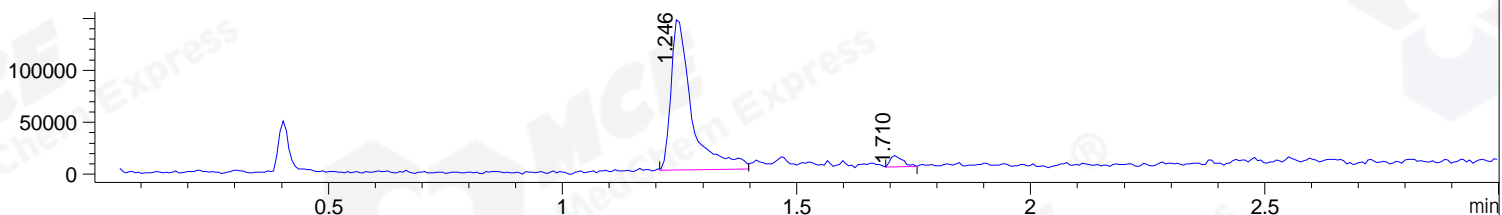

Ion 344, MSD1 344, Target Mass 343 +H Positive, EIC=343.7:344.7

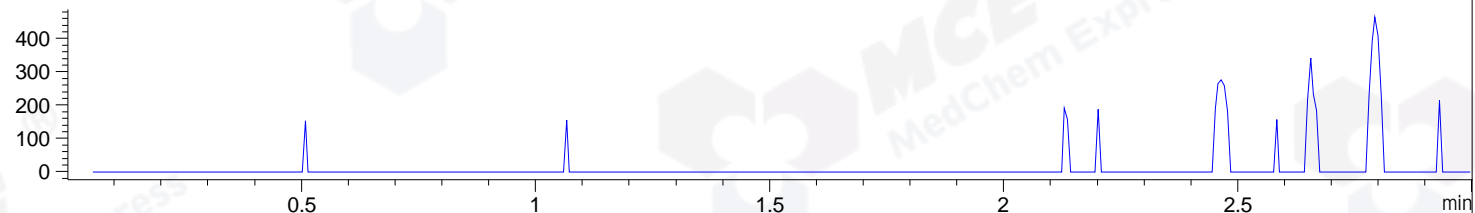

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.24	0.03	506.37	294.60	98.82	254
1.46	0.02	1.61	1.78	0.31	254
1.70	0.02	4.45	3.84	0.87	254

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.24	0.03	1909.22	1080.28	99.62	254
1.46	0.02	6.41	6.14	0.33	254
1.70	0.01	0.96	1.18	0.05	254

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.25	0.04	442049.28	147333.77	95.82	254
1.71	0.03	19277.59	10386.48	4.18	254

Ret. Time: 1.25

<<<< POSITIVE SPECTRA >>>>

ES-API Positive



Ret. Time: 1.71

ES-API Positive

