


=====
Acq. Operator : Su Xiao Ying(LCMS-02) Seq. Line : 76
Acq. Instrument : HY-LCMS-02 Location : P1-B-07
Injection Date : 4/8/2016 2:50:29 PM Inj : 1
Inj Volume : 3.000 µl
Different Inj Volume from Sample Entry Actual Inj Volume : 8.000 µl
Acq. Method : D:\AGLIENT 1260\DATA\20160408\20160408 2016-04-08 08-38-27\100-1000MS+3MIN-1.5_(0.02%FA).M
Last changed : 4/8/2016 8:38:27 AM by Su Xiao Ying(LCMS-02)
Analysis Method : D:\AGLIENT 1260\DATA\20160408\20160408 2016-04-08 08-38-27\100-1000MS+3MIN-1.5_(0.02%FA).M (Sequence Method)
Last changed : 4/8/2016 3:17:30 PM by Su Xiao Ying(LCMS-02)
(modified after loading)
Method Info : HY-365_5H01RS,M,A-RP-108, 210nm,23min

Catalog No : HY-D0150 Batch#20039
A-RP-134

Additional Info : Peak(s) manually integrated
DAD1 B, Sig=214,4 Ref=off (D:\AGLIENT...0\DATA\20160408\20160408 2016-04-08 08-38-27\BIZ2016-408-WJ8-1.D)

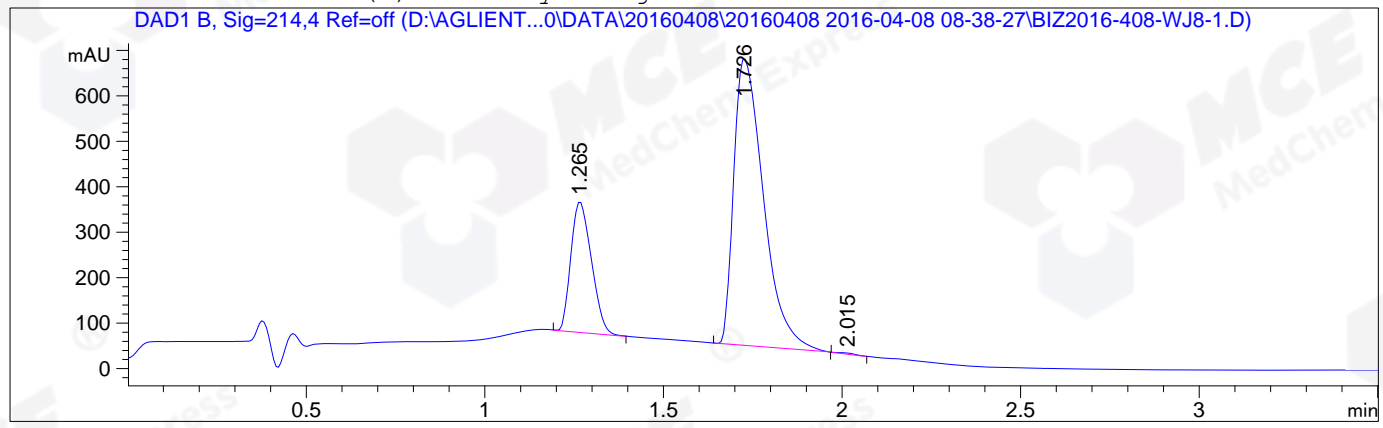

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 B, Sig=214,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	1.265	MM	0.0664	1153.06055	289.26004	24.0250
2	1.726	MM	0.0960	3637.68506	631.48956	75.7944
3	2.015	MM	0.0528	8.66475	2.73293	0.1805

Totals : 4799.41035 923.48254


=====
*** End of Report ***

=====

Acq. Operator	: Su Xiao Ying(LCMS-02)	Seq. Line	: 76
Acq. Instrument	: HY-LCMS-02	Location	: P1-B-07
Injection Date	: 4/8/2016 2:50:29 PM	Inj	: 1
		Inj Volume	: 3.000 µl
Different Inj Volume from Sample Entry		Actual Inj Volume	: 8.000 µl
Method	: D:\AGLIENT 1260\DATA\20160408\20160408 2016-04-08 08-38-27\100-1000MS+3MIN-1.5_(0.02%FA).M (Sequence Method)		
Last changed	: 4/8/2016 8:38:27 AM by Su Xiao Ying(LCMS-02)		
Method Info	: HY-365_5H01RS,M,A-RP-108, 210nm,23min		


Catalog No : HY-D0150 Batch#20039
A-RP-134

Additional Info : Peak(s) manually integrated

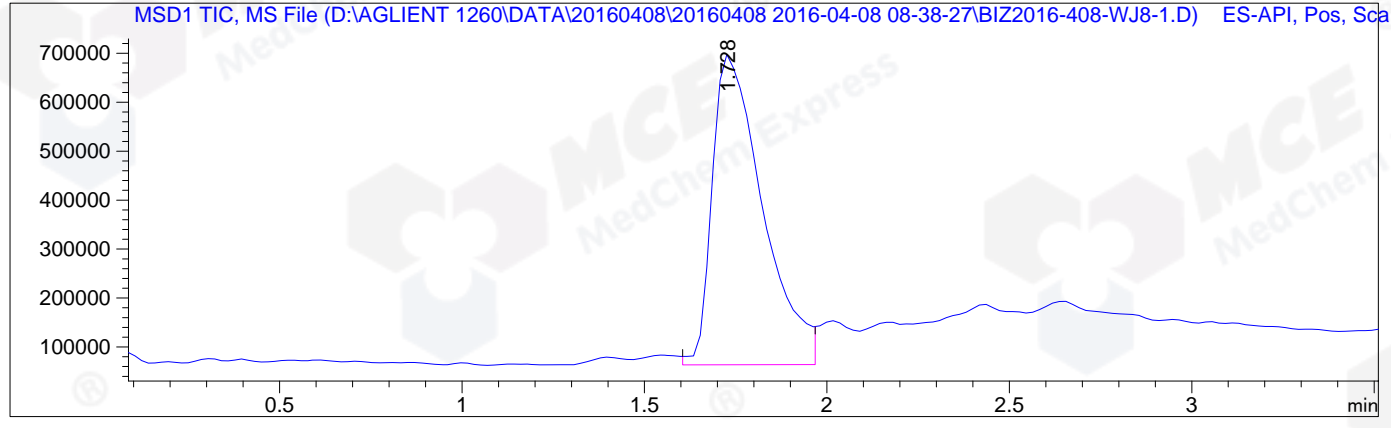

MS Signal: MSD1 TIC, MS File, ES-API, Pos, Scan, Frag: 50
Spectra averaged over upper half of peaks.
Noise Cutoff: 1000 counts.
Reportable Ion Abundance: > 10%.

Retention Time (MS)	MS Area	Mol. Weight or Ion
1.728	6074122	306.15 I 305.15 I

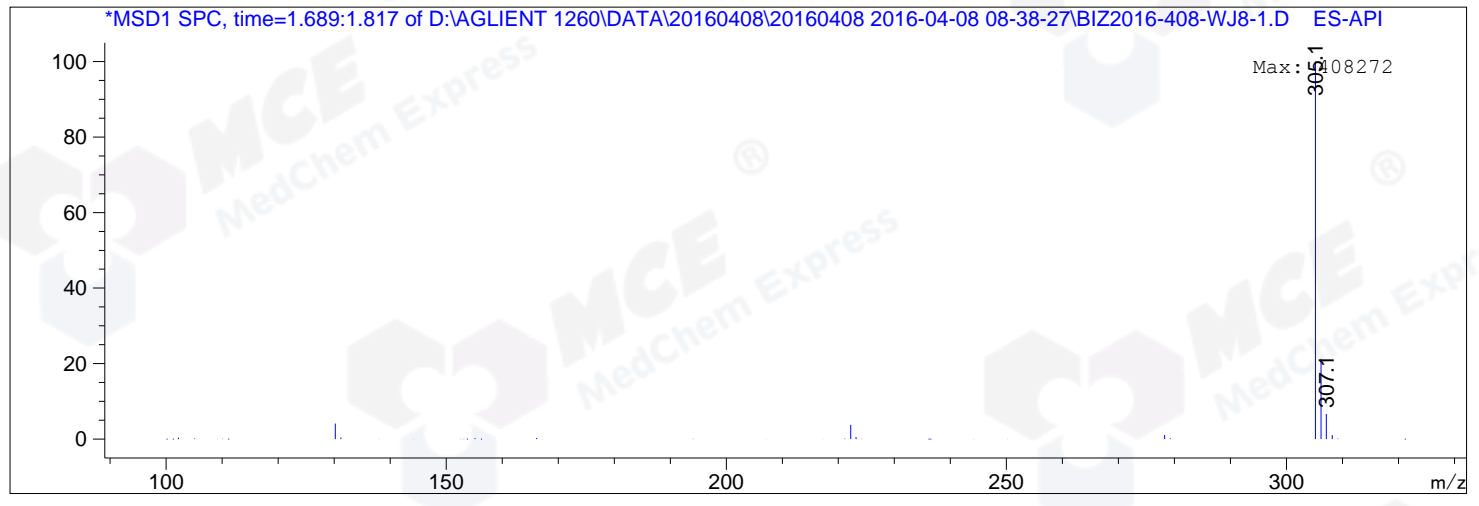

*** End of Report ***