



File ..1\DATA\2019\20190424\558\BIZ2019-423-WYQ1.D Tgt Mass (CHM):
 Injection Date : 24 Apr 19 11:08 am +0800 Seq. Line : 22
 Sample Name : BIZ2019-423-WYQ1 Location : P2-B-09
 Acq. Operator : LQ_1052 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2019\20190424\558\1-POS-3MIN-1.M
 Analysis Method : D:\CHEM32\1\DATA\2019\20190424\558\1-POS-3MIN-1.M
 Catalog No : HY-N0141 Batch#40463
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-322
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

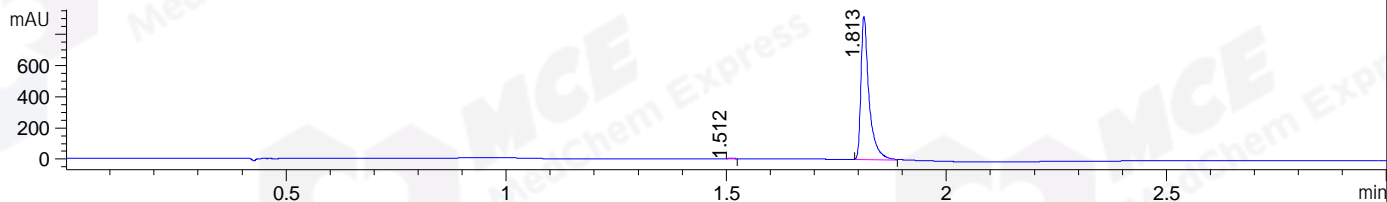


DAD1 C, Sig=254,4 Ref=off

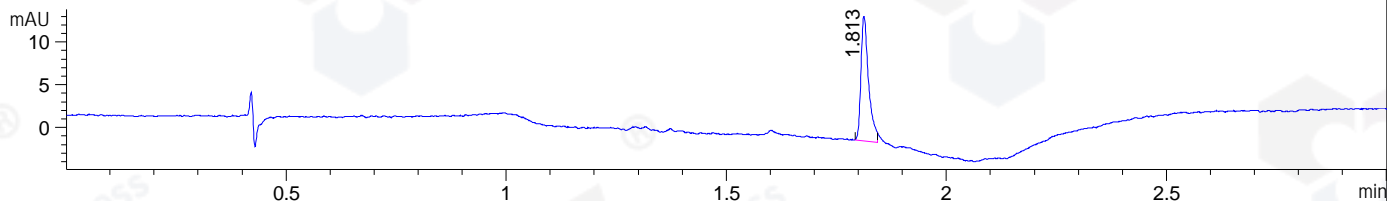

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

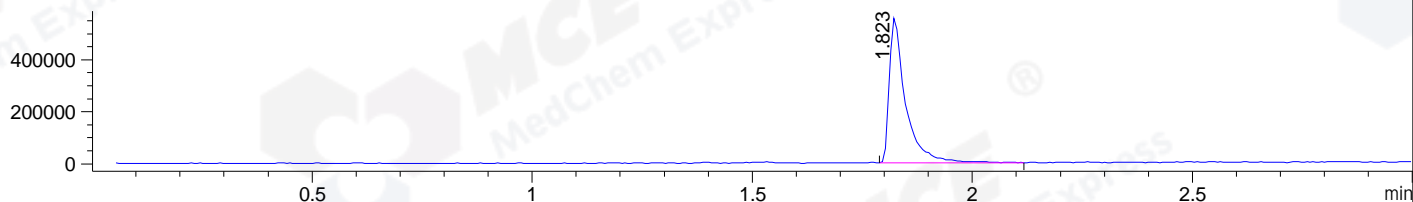

Ion 249.1, MSD1 249.1, Target Mass 248.1 +H Positive, EIC=248.8:249.8

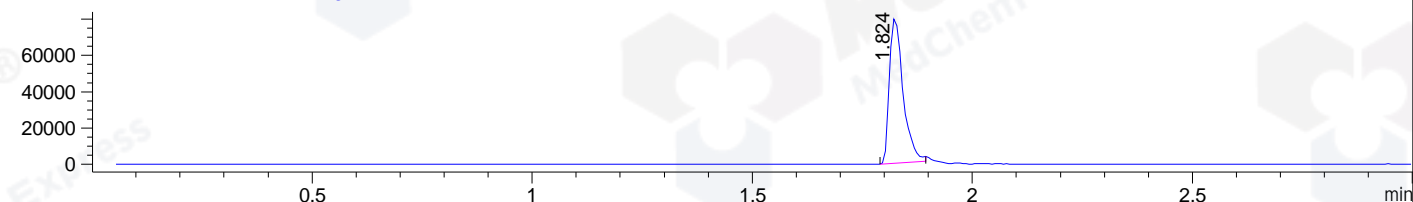

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.51	0.01	1.38	1.77	0.12	ND
1.81	0.02	1172.04	916.34	99.88	231

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.81	0.02	17.56	14.58	100.00	231

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.82	0.04	1447632.00	561786.06	100.00	231

Ret. Time: 1.82

<<<< POSITIVE SPECTRA >>>>

