



File ..DATA\2020\20200311\868\CPK2020-311-22711-.D Tgt Mass (CHM):  
 Injection Date : 13 Mar 20 2:38 am +0800 Seq. Line : 113  
 Sample Name : CPK2020-311-22711 Location : P1-C-02  
 Acq. Operator : ZJ\_1432 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 0.5 ul  
 Acq. Method : D:\Chem32\1\data\2020\20200311\868\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2020\20200311\868\1-POS-3MIN.M  
 Catalog No : HY-N0226A Batch#22711  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-433  
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

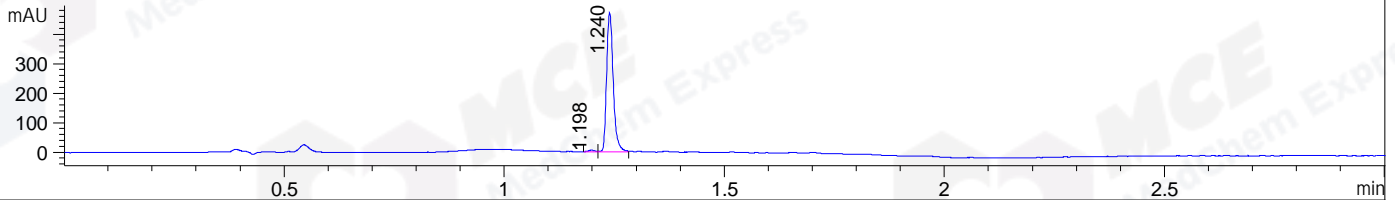


DAD1 C, Sig=254,4 Ref=off

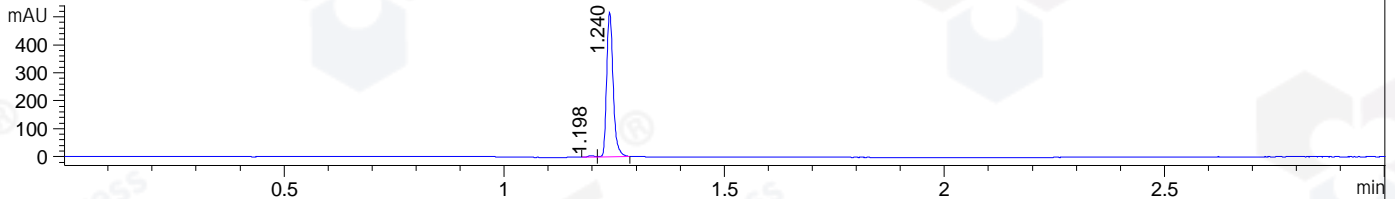

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

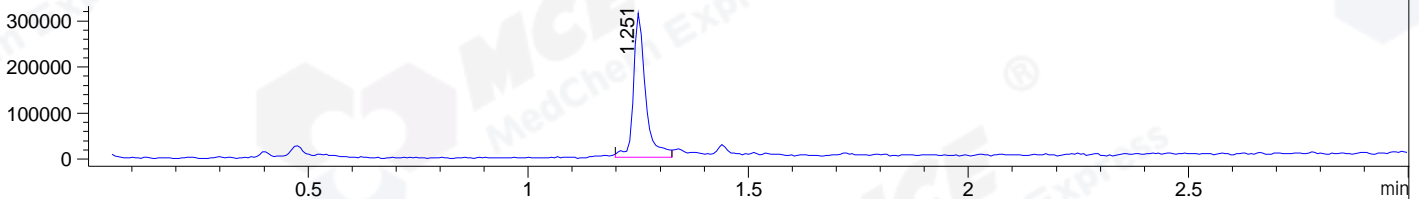

Ion 372, MSD1 372, Target Mass 371 +H Positive, EIC=371.7:372.7

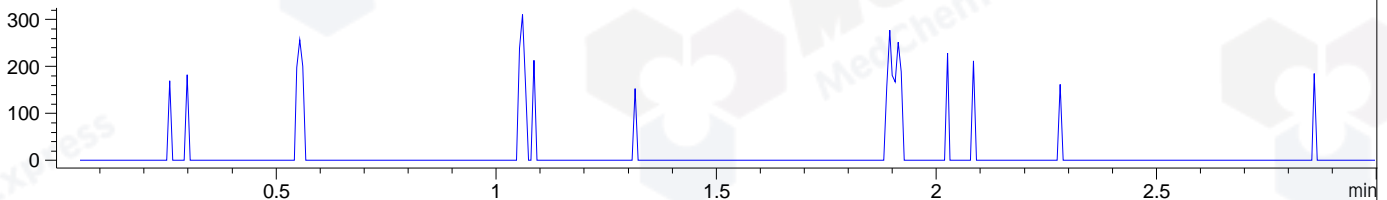

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.20	0.02	5.52	5.46	1.11	322
1.24	0.02	490.07	471.37	98.89	336

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.20	0.02	6.08	5.57	1.13	322
1.24	0.02	531.05	517.69	98.87	336

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.25	0.03	597868.94	313199.88	100.00	336

Ret. Time: 1.25

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

