



File ..DATA\2020\20200923\1115\CPK2020-922-28182.D Tgt Mass (CHM):  
 Injection Date : 23 Sep 20 7:32 pm +0800 Seq. Line : 116  
 Sample Name : CPK2020-922-28182 Location : PL-A-08  
 Acq. Operator : zyj\_1547 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2020\20200923\1115\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2020\20200923\1115\1-POS-3MIN.M  
 Catalog No : HY-N0360  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-624


DAD1 B, Sig=214,4 Ref=off

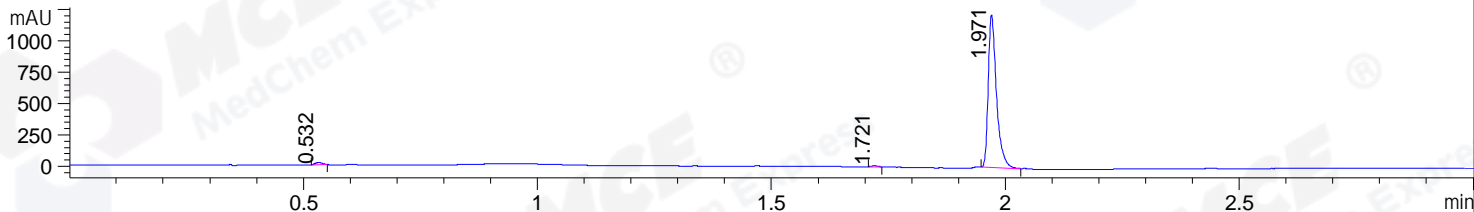


DAD1 C, Sig=254,4 Ref=off

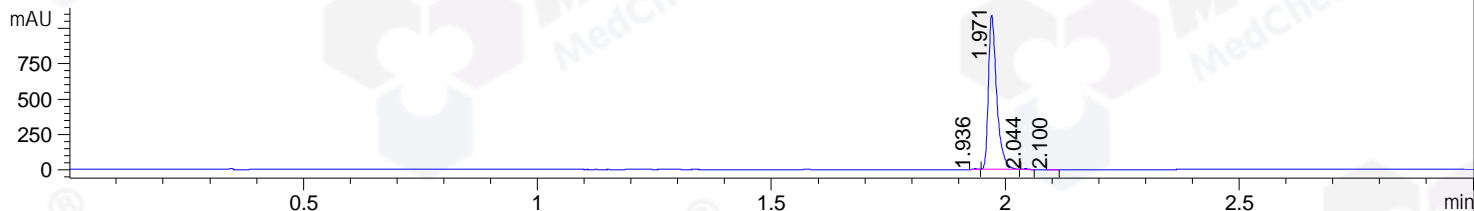

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

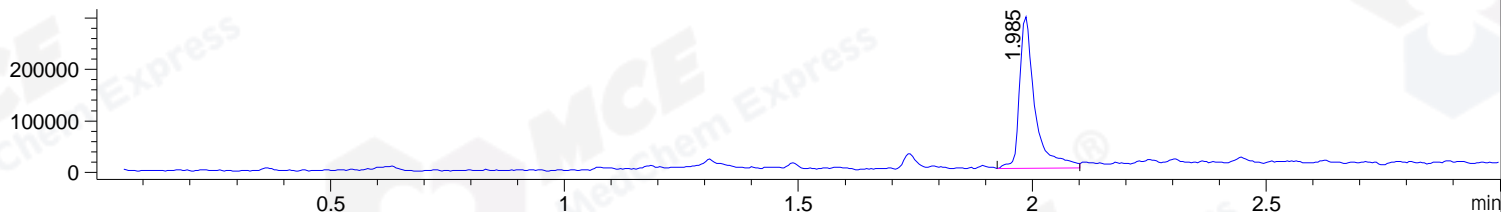

Ion 279, MSD1 279, Target Mass 278 +H Positive, EIC=278.7:279.7

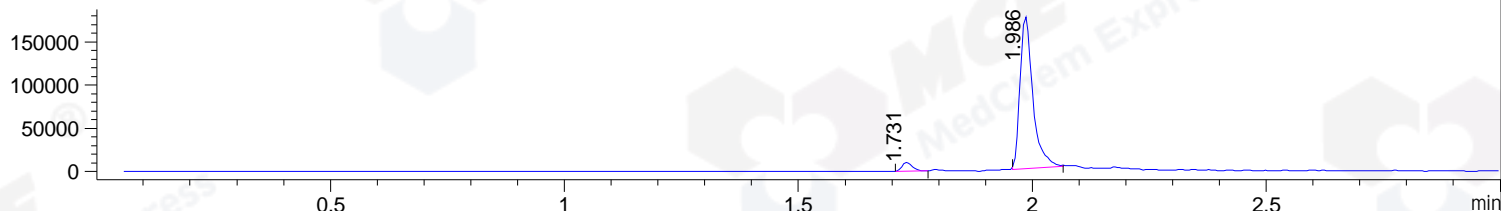

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
0.53	0.02	18.98	17.37	1.25	166
1.72	0.02	7.40	7.93	0.49	279
1.97	0.02	1491.01	1219.26	98.26	279

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.94	0.01	3.90	5.34	0.29	279
1.97	0.02	1347.45	1094.20	99.22	279
2.04	0.01	4.20	5.21	0.31	279
2.10	0.01	2.52	2.85	0.19	279

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.99	0.03	676497.06	295105.66	100.00	279

Ret. Time: 1.99

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

