



File ..\DATA\2019\20190823\705\CPK2019-822-22728.D Tgt Mass (CHM):
 Injection Date : 24 Aug 19 9:21 am +0800 Seq. Line : 5
 Sample Name : CPK2019-822-22728 Location : P1-B-08
 Acq. Operator : ZJ_1432 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 5 ul
 Acq. Method : D:\Chem32\1\data\2019\20190823\705\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2019\20190823\705\1-POS-3MIN.M
 Catalog No : HY-N0417 Batch#22728
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

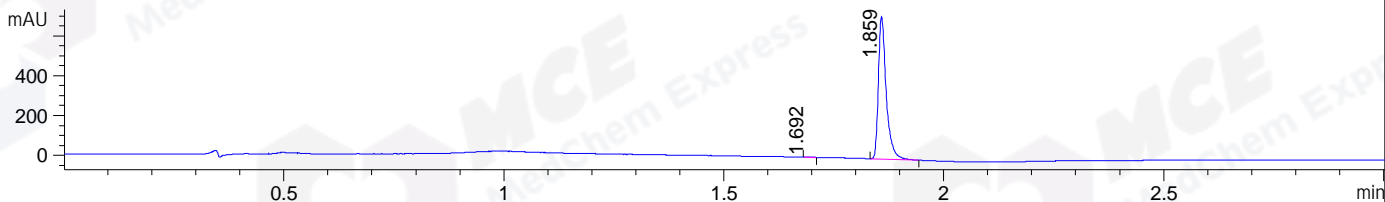


DAD1 C, Sig=254,4 Ref=off

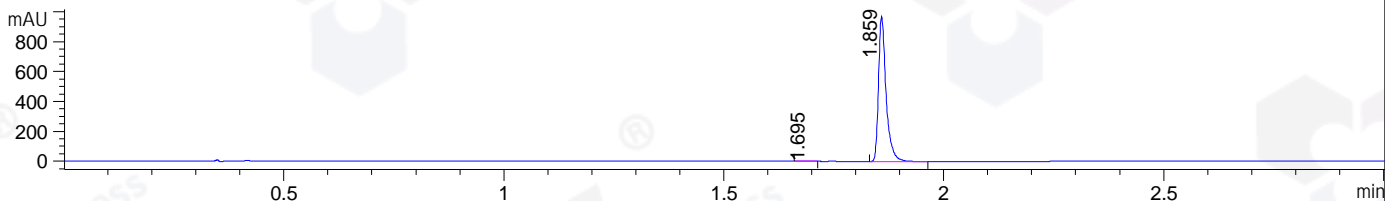

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

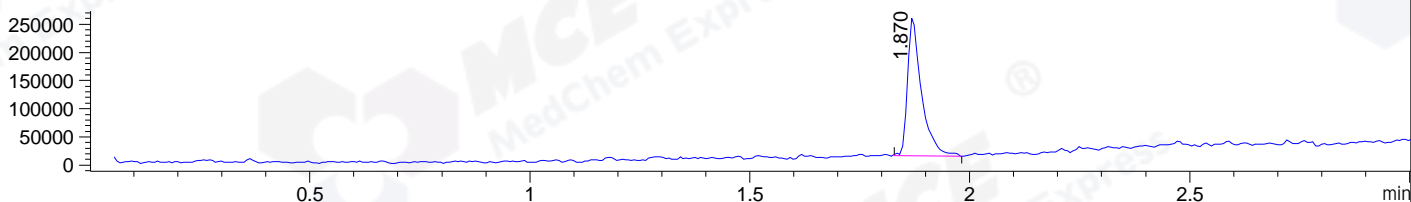

Ion 557.7027, MSD1 557.7027, Target Mass 556.7027 +H Positive, EIC=557.40:558.40

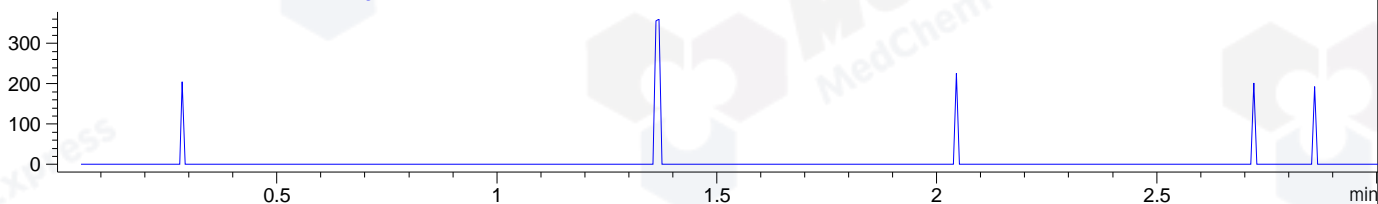

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.69	0.01	1.37	1.56	0.15	141
1.86	0.02	884.15	716.02	99.85	497

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.69	0.02	0.96	0.66	0.08	141
1.86	0.02	1161.61	971.97	99.92	579

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.87	0.03	545032.38	248803.25	100.00	579

Ret. Time: 1.87

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

