


Software Version : 6.3.1.0504  
Sample Name : LJ1708020143 1039550  
Instrument Name : CLARUS 600  
Rack/Vial : 0/17  
Sample Amount : 1.000000  
Cycle : 1  
Catalog No : HY-N0445 Batch# 40511

Date : 2017-8-10 10:22:10  
Data Acquisition Time : 2017-8-9 15:52:21  
Channel : A  
Operator : manager  
Dilution Factor : 1.000000

Result File :  
Sequence File : D:\sequence\170809.seq

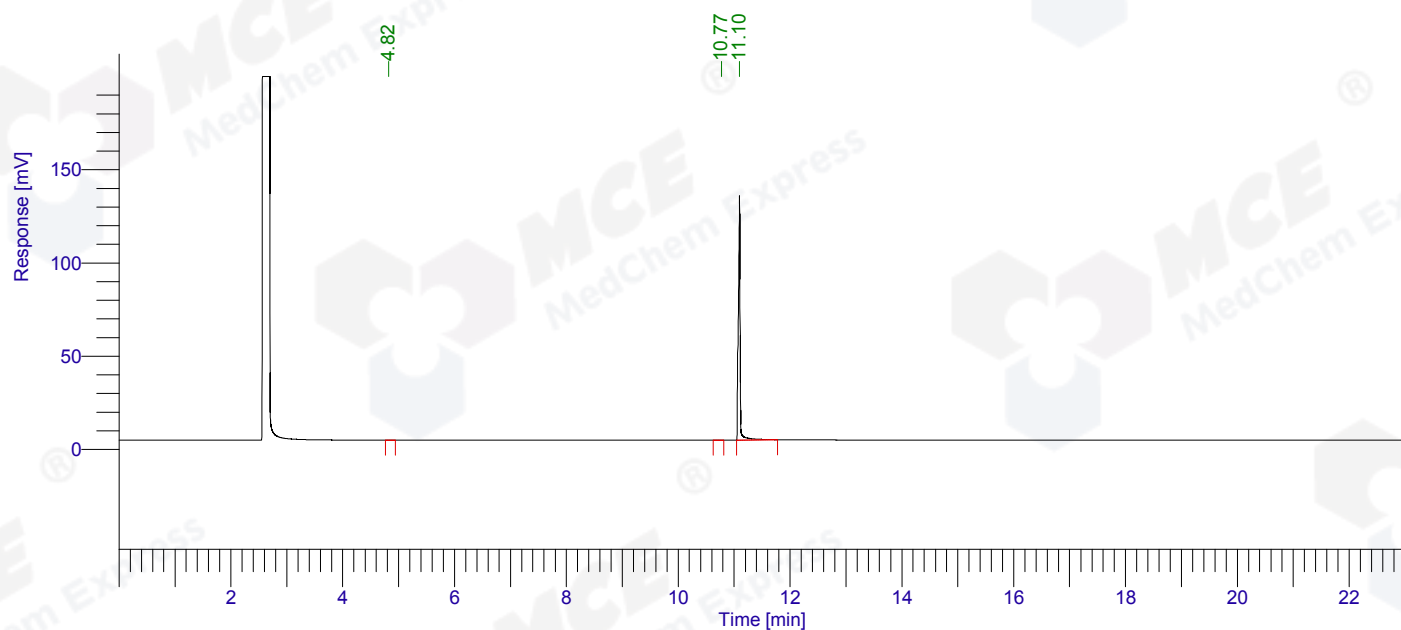

## Area Percent Report

Peak #	Component Name	Time [min]	Area [UV*sec]	Area Percent [%]
1		4.819	125.79	0.0425
2		10.773	155.10	0.0523
3		11.099	296016.06	99.9052
			296296.95	100.0000

Missing Component Report  
Component Expected Retention (Calibration File)

All components were found