

File ..1\DATA\2019\20190117\552\BIZ2019-116-WYQ5.D Tgt Mass (CHM):

Injection Date : 17 Jan 19 10:57 am +0800 Seq. Line : 19

Sample Name : BIZ2019-116-WYQ5 Location : P2-C-01

Acq. Operator : LQ_1052 Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\Chem32\1\data\2019\20190117\552\1-POS-3MIN-1.M

Analysis Method : D:\CHEM32\1\DATA\2019\20190117\552\1-POS-3MIN-1.M

Catalog No : HY-N0637 Batch#36881

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-314

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

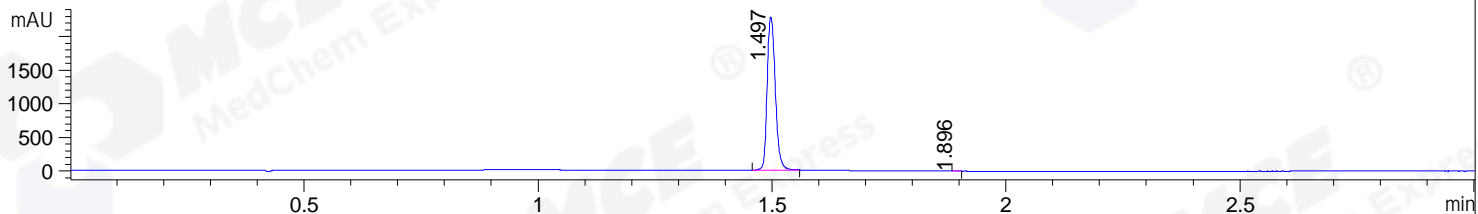


DAD1 C, Sig=254,4 Ref=off

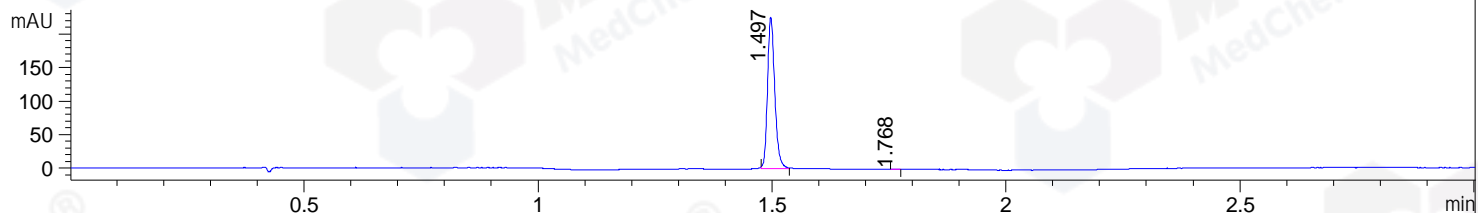

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

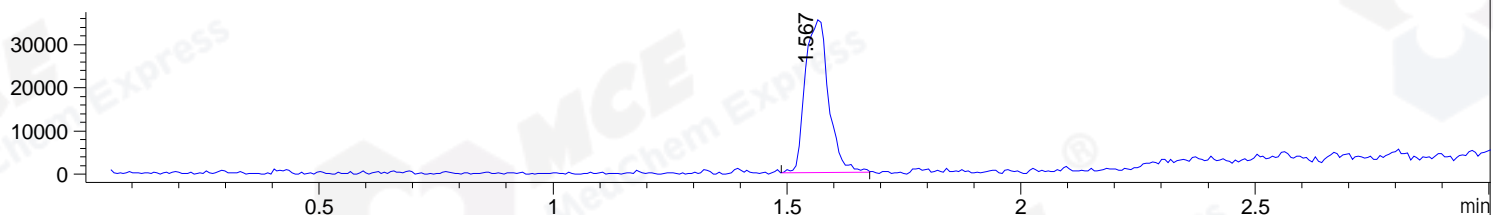

Ion 289, MSD1 289, Target Mass 288 +H Positive, EIC=288.7:289.7

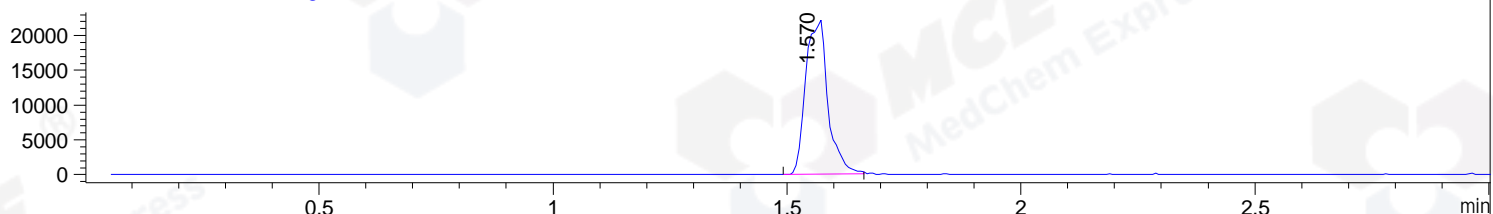

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.50	0.02	2781.96	2282.53	99.98	289
1.90	0.01	0.53	0.82	0.02	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.50	0.02	243.46	226.09	99.87	289
1.77	0.01	0.33	0.39	0.13	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.57	0.06	123269.52	35449.14	100.00	289

Ret. Time: 1.57

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

