



File ..DATA\2021\20210126\1250\CPK2021-125-18937.D Tgt Mass (CHM):  
Injection Date : 26 Jan 21 9:06 pm +0800 Seq. Line : 128  
Sample Name : CPK2021-125-18937 Location : P1-D-08  
Acq. Operator : yrz\_1364 Inj : 1  
Spec. Reported : MS Integration Inj Volume : 1 ul  
Acq. Method : D:\Chem32\1\data\2021\20210126\1250\1-POS-3MIN.M  
Analysis Method : D:\CHEM32\1\DATA\2021\20210126\1250\1-POS-3MIN.M  
CAS NO. : 906-33-2  
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
Gradient: 5% to 95%B within 1.3 min  
Flow Rate :1.8ml/min  
Column :SunFire C18, 4.6\*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

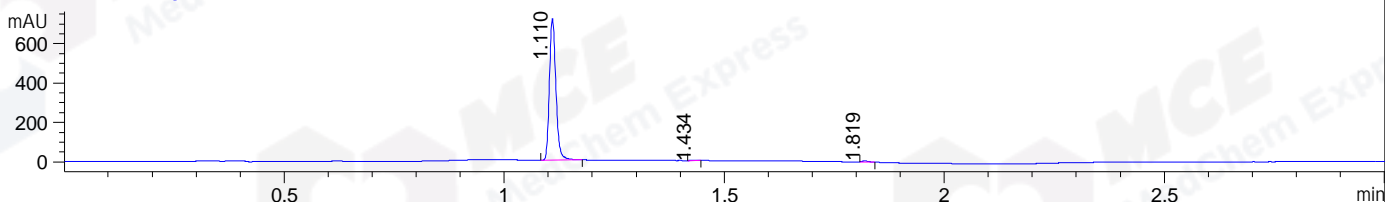


DAD1 C, Sig=254,4 Ref=off

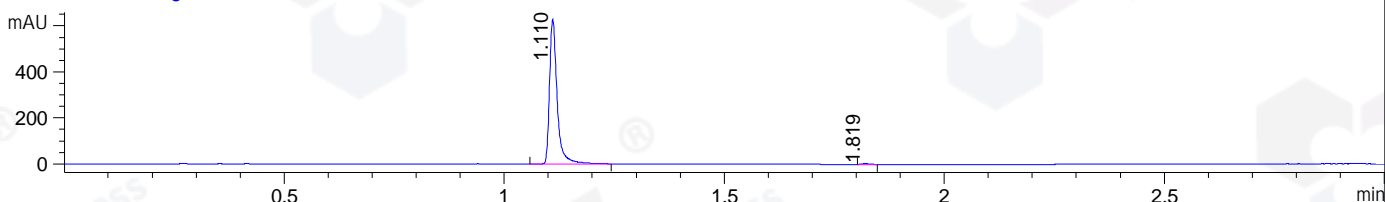

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

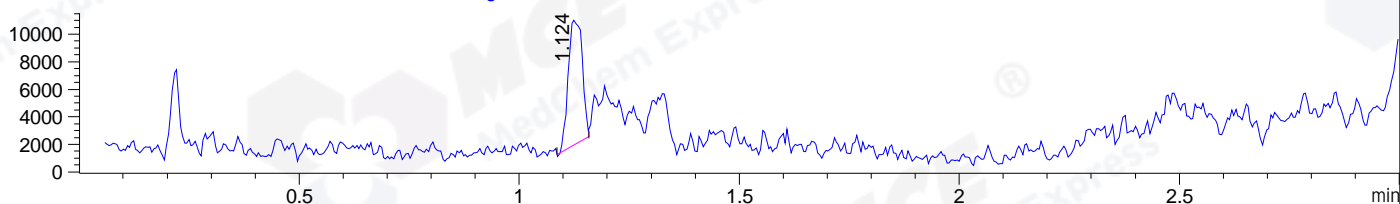

Ion 355, MSD1 355, Target Mass 354 +H Positive, EIC=354.7:355.7

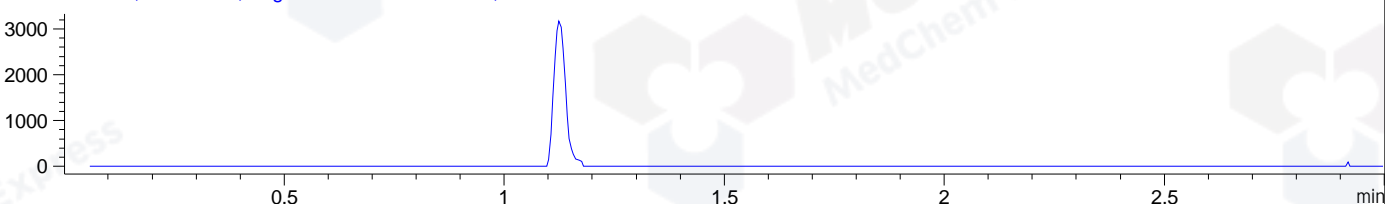

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.11	0.02	737.35	719.54	99.07	163
1.43	0.01	1.31	1.65	0.18	ND
1.82	0.02	5.64	5.67	0.76	ND

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.11	0.02	762.72	628.98	99.44	ND
1.82	0.02	4.30	3.71	0.56	ND

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.12	0.03	19897.15	9051.51	100.00	163

Ret. Time: 1.12

<<<< POSITIVE SPECTRA >>>>

