
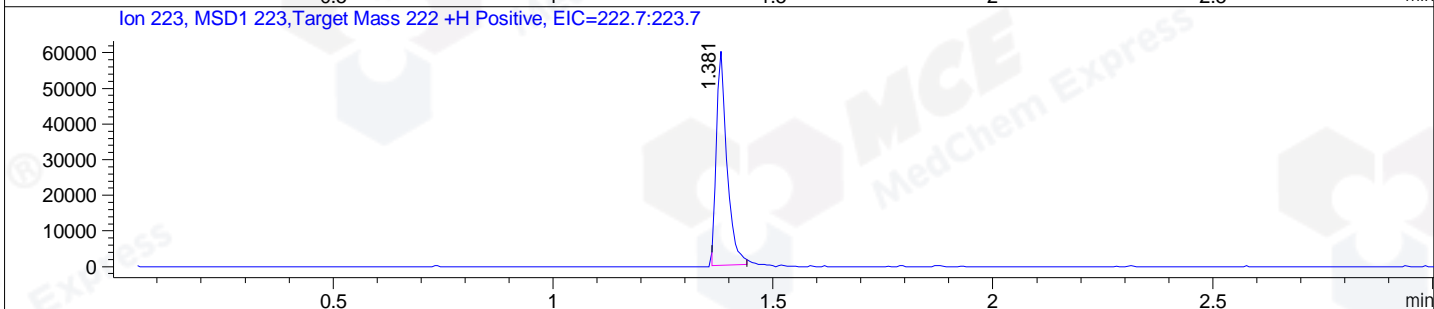
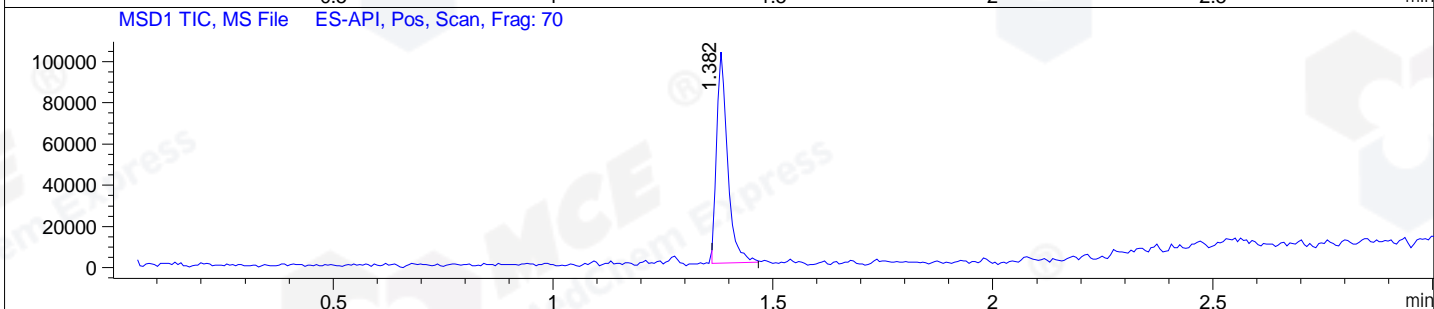


File ..1\DATA\2020\20200508\949\BIZ2020-506-SCH3.D Tgt Mass (CHM):
 Injection Date : 8 May 20 9:16 am +0800 Seq. Line : 7
 Sample Name : BIZ2020-506-SCH3 Location : P1-A-08
 Acq. Operator : ZJ_1432 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 0.25 ul
 Acq. Method : D:\Chem32\1\data\2020\20200508\949\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200508\949\1-POS-3MIN.M
 Catalog No : HY-N0774
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-607
 Oven Temperature : 45

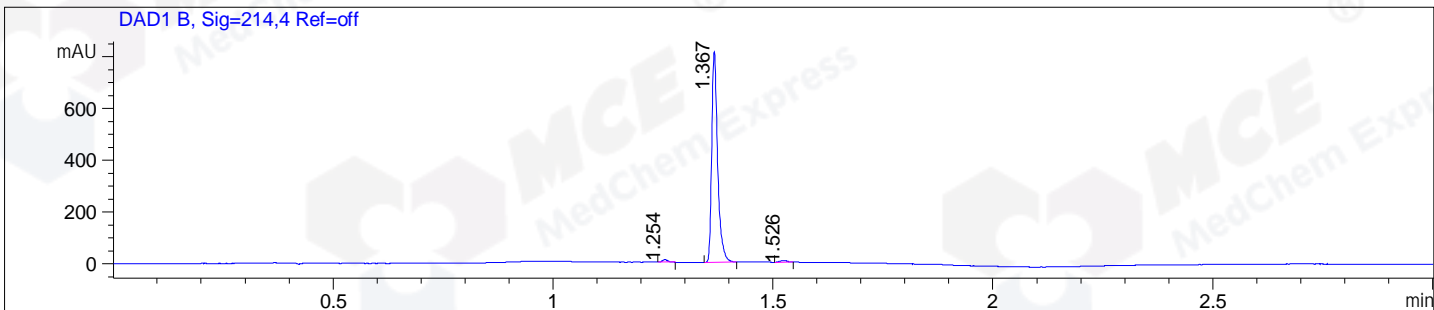

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.25	0.01	7.45	9.43	0.97	ND
1.37	0.02	756.75	813.20	98.14	223
1.53	0.02	6.88	6.19	0.89	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.38	0.03	178471.81	102379.74	100.00	223

Ret. Time: 1.38

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

