

File ..\DATA\2020\20200829\1090\BIZ2020-828-WLQ1.D Tgt Mass (CHM):

Injection Date : 29 Aug 20 10:25 am +0800 Seq. Line : 19

Sample Name : BIZ2020-828-WLQ1 Location : PL-B-06

Acq. Operator : zyj\_1547 Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\Chem32\1\data\2020\20200829\1090\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2020\20200829\1090\1-POS-3MIN.M

Catalog No : HY-N1196

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6\*50mm,3.5um A-RP-607

Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

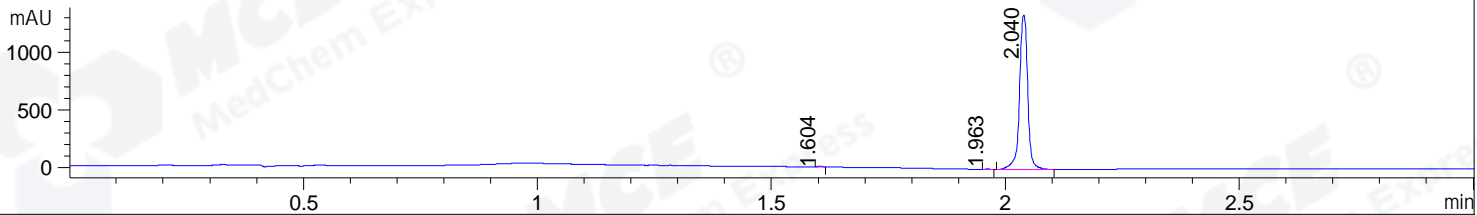


DAD1 C, Sig=254,4 Ref=off

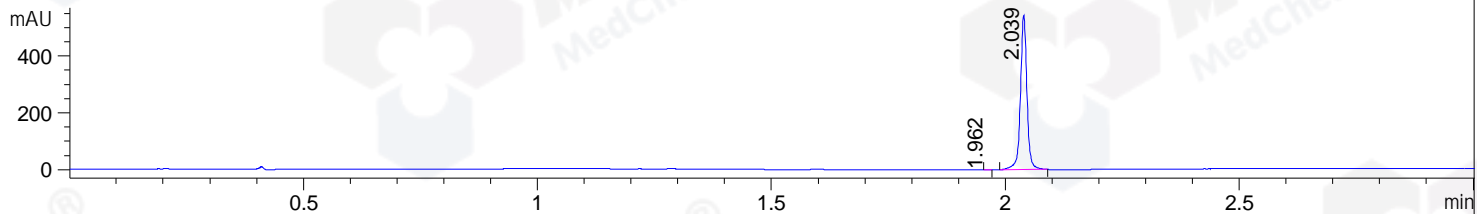

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

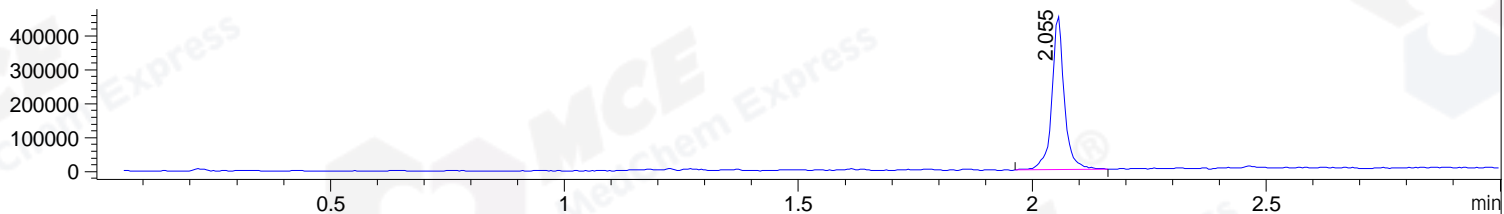

Ion 245, MSD1 245, Target Mass 244 +H Positive, EIC=244.7:245.7

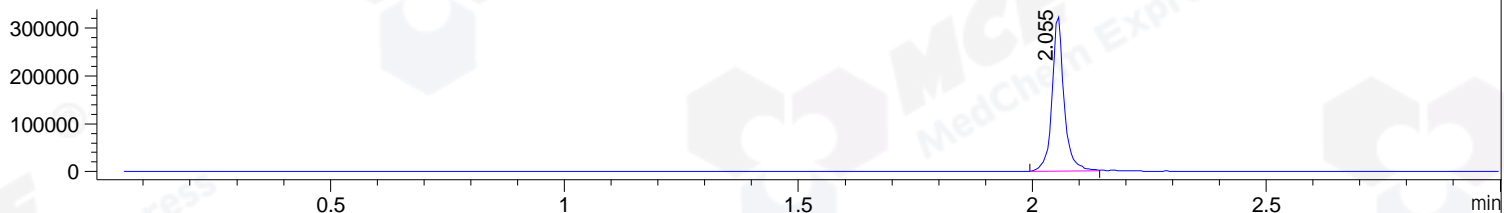

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.60	0.01	3.73	5.13	0.23	177
1.96	0.01	2.65	3.96	0.16	ND
2.04	0.02	1647.52	1343.34	99.61	245

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.96	0.01	0.46	0.80	0.09	ND
2.04	0.02	527.86	543.97	99.91	245

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
2.05	0.03	839535.44	453578.19	100.00	245

Ret. Time: 2.05

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

