



File ..DATA\2020\20200615\995\CPK2020-608-26446-.D Tgt Mass (CHM):
 Injection Date : 15 Jun 20 2:17 pm +0800 Seq. Line : 60
 Sample Name : CPK2020-608-26446 Location : P1-C-05
 Acq. Operator : ZJ_1432 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 0.5 ul
 Acq. Method : D:\Chem32\1\data\2020\20200615\995\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200615\995\1-POS-3MIN.M
 Catalog No : HY-N1394
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-607
 Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

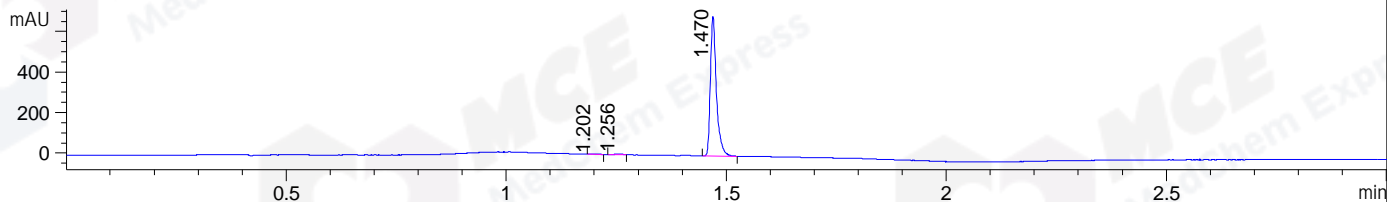


DAD1 C, Sig=254,4 Ref=off

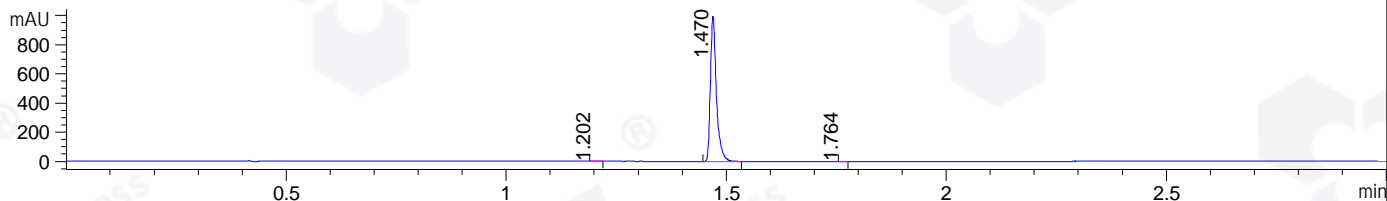

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

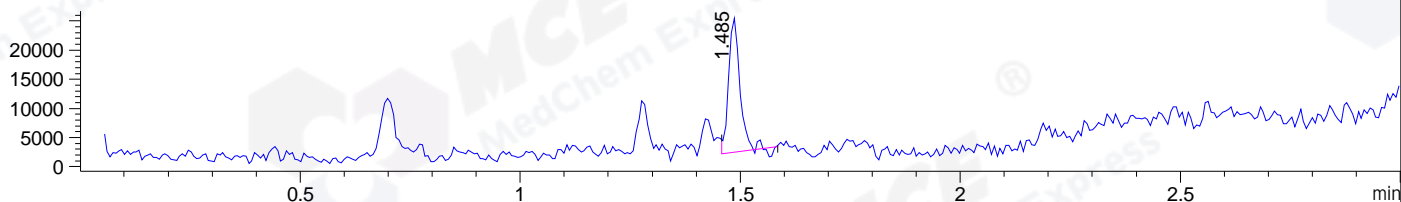

Ion 153, MSD1 153, Target Mass 152 +H Positive, EIC=152.7:153.7

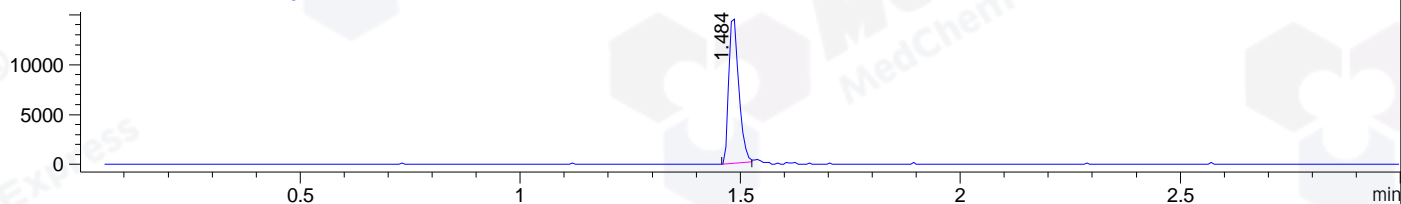

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.20	0.02	1.99	1.73	0.30	ND
1.26	0.02	4.06	3.51	0.61	340
1.47	0.02	656.94	689.88	99.09	153

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.20	0.01	1.48	1.92	0.16	ND
1.47	0.02	945.12	998.86	99.81	153
1.76	0.01	0.34	0.55	0.04	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.49	0.03	39755.23	23178.66	100.00	153

Ret. Time: 1.49

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

