


Catalog No: HY-N2342 Batch#46951

Chromatographic Column : ODS-C18-250*4.6mm,5um : 280
 Moving Phase :Acetonitrile : 0.2%Phosphoric Solution Temper : 30°
 Flow Velocity : 1ml/min Pressure :10Mpa
 :Gradient : Acetonitrile=8%~18% , 15min

Autostop : 20.00 min

Detector1 : 1.

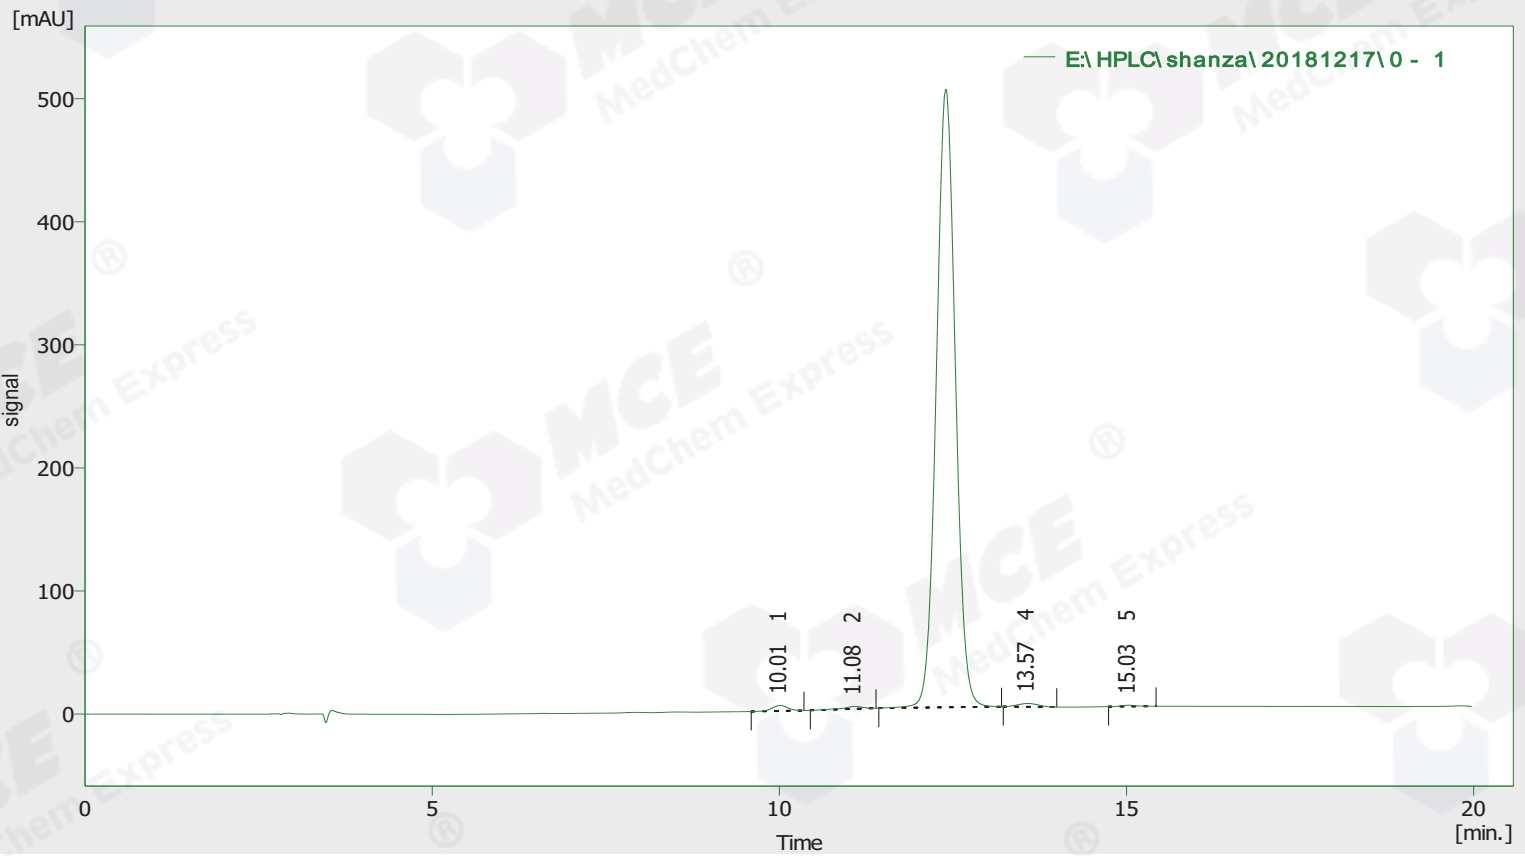

Result(- E:\HPLC\shanza\20181217\0 - 1)

	Ret time [min]	Area [mAU.s]	Hieght [mAU]	Area [%]	Hieght [%]	W05 [min]
1	10.008	68.698	4.469	0.7	0.9	0.24
2	11.081	40.710	2.044	0.4	0.4	0.27
3	12.398	9566.383	502.033	98.2	98.0	0.29
4	13.574	57.059	2.746	0.6	0.5	0.34
5	15.033	13.845	0.983	0.1	0.2	0.22
	Totals	9746.693	512.276	100.0	100.0	