



File ..\DATA\2020\20200715\1037\BIZ2020-713-SCH4.D Tgt Mass (CHM):  
 Injection Date : 15 Jul 20 9:20 am +0800 Seq. Line : 4  
 Sample Name : BIZ2020-713-SCH4 Location : P1-C-05  
 Acq. Operator : ZJ\_1432 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 0.3 ul  
 Acq. Method : D:\Chem32\1\data\2020\20200715\1037\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2020\20200715\1037\1-POS-3MIN.M  
 Catalog No : HY-N2435  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-607  
 Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

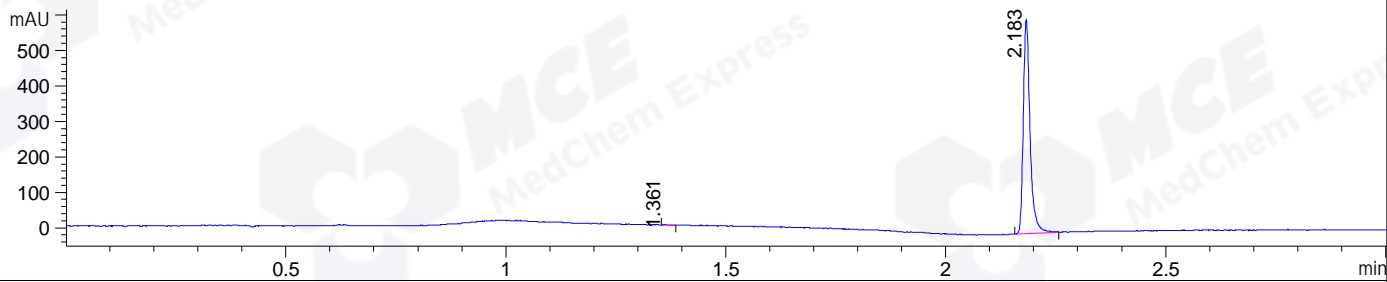

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

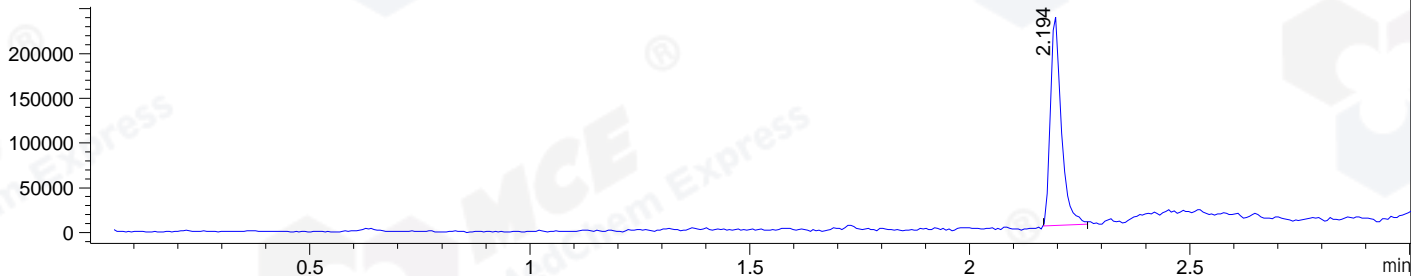

Ion 305, MSD1 305, Target Mass 304 +H Positive, EIC=304.7:305.7

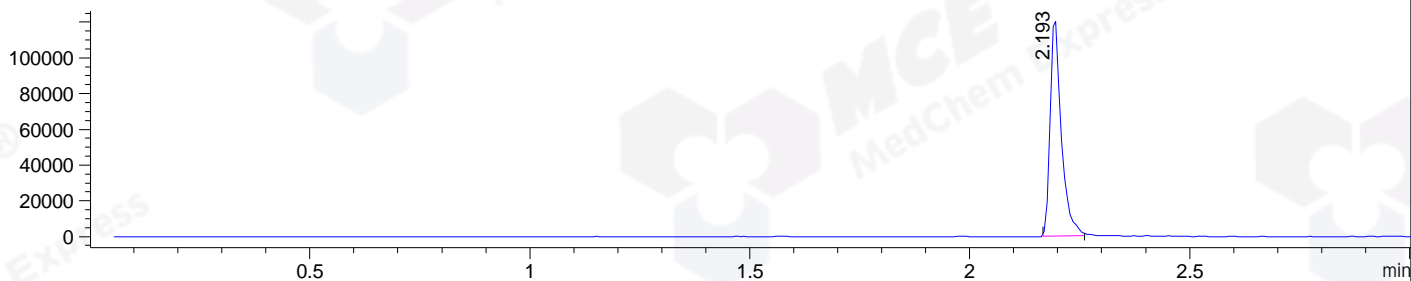

Integration Results for DAD1 B, Sig=214,4 Ref=off

| RetTim | Width | Area   | Height | Area% | MS (+) |
|--------|-------|--------|--------|-------|--------|
| 1.36   | 0.01  | 1.71   | 1.90   | 0.26  | ND     |
| 2.18   | 0.02  | 643.41 | 602.31 | 99.74 | 305    |

Integration Results for MSD1 TIC, MS File

| RetTim | Width | Area      | Height    | Area%  | MS (+) |
|--------|-------|-----------|-----------|--------|--------|
| 2.19   | 0.03  | 409410.03 | 236485.97 | 100.00 | 305    |

Ret. Time: 2.19

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

