


## SAMPLE INFORMATION

Sample Name:		Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	
Vial:	88	Acq. Method Set:	$\beta$ -Crocetin
Injection #:	1	Processing Method:	Samples
Injection Volume:	10.00 $\mu$ l	Channel Name:	443.0nm
Run Time:	25.0 Minutes	Proc. Chnl. Descr.:	PDA 443.0 nm
Catalog No:	HY-N6904 Batch#57253		
Date Acquired:	2018-8-16 14:12:05 CST		
Date Processed:	2018-8-16 14:40:48 CST		

### Auto-Scaled Chromatogram

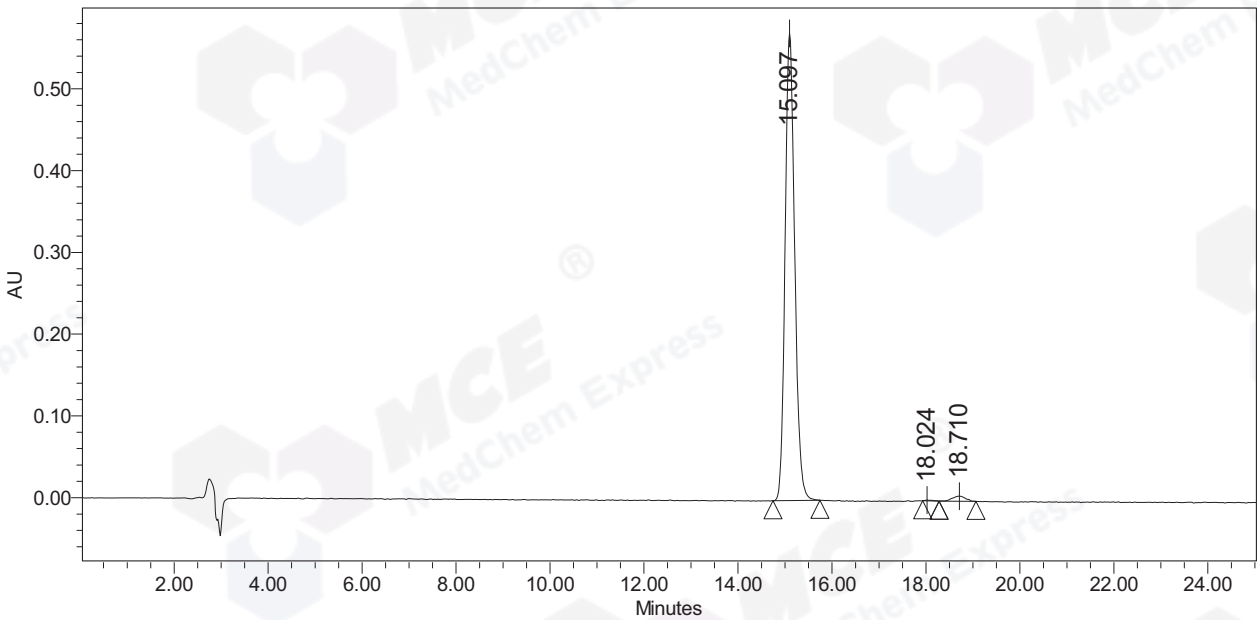

### Peak Results

Name	RT	Area	% Area	USP Plate Count	USP Resolution
1	15.097	8104094	98.41	26230.04	
2	18.024	11464	0.14	71784.25	9.02
3	18.710	119307	1.45	19629.69	1.69