

Data file: C:\CHEM32\1\DATA\200826\200826 2020-08-26 16-40-59\HY-P0122.D

Catalog No: HY-P0122

Description: Mobile phase: Buffer A: 0.1% TFA in H₂O
Buffer B: 0.1% TFA in ACN
Gradient: 0-25% B in 25min, Flow rate: 1.0ml/min
Column: Unitary C18, 4.6*150mm, 5um 100A (A-007)
Instrument: Agilent HPLC 1100

Instrument: 1100

Location: 25


Injection date: 2020/8/26 19:21:19

Injection: 1 of 1

Last changed: 2020/8/27 16:15:15

Injection volume: 10.000

Acq. operator: qc

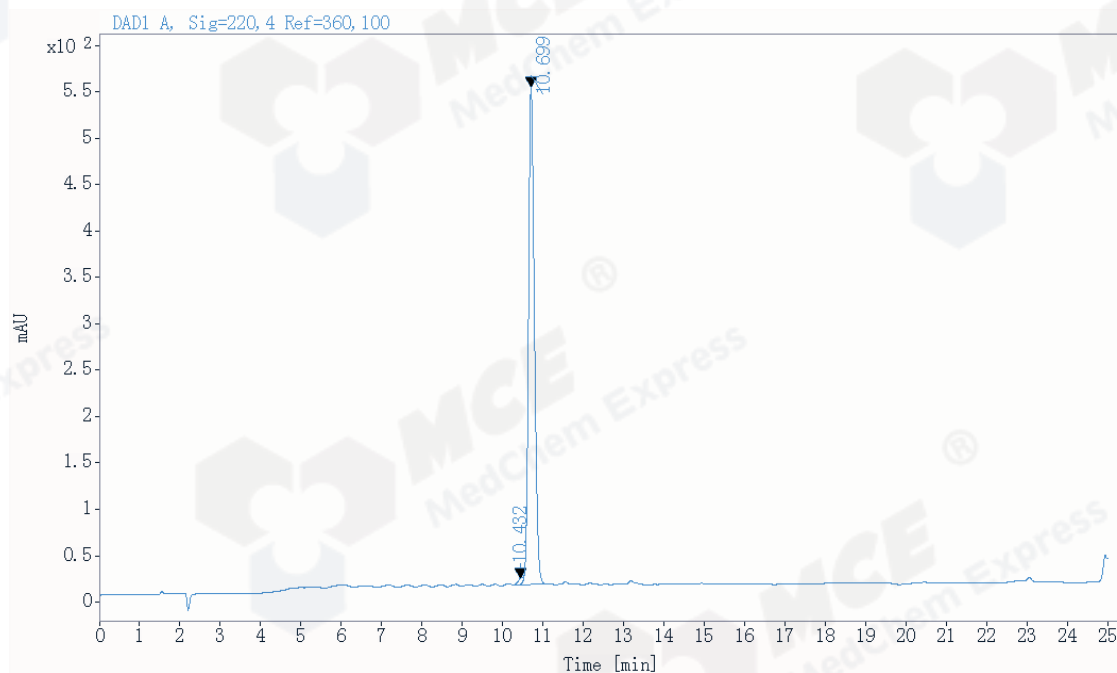

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[min]	Type	Width[min]	Area	Height	Area% Name
10.432	BV E	0.1205	54.0466	6.5329	0.9696
10.699	VB R	0.1600	5519.8486	536.7387	99.0304
	Sum		5573.8952		