


### MASS SPECTROMETRY REPORT

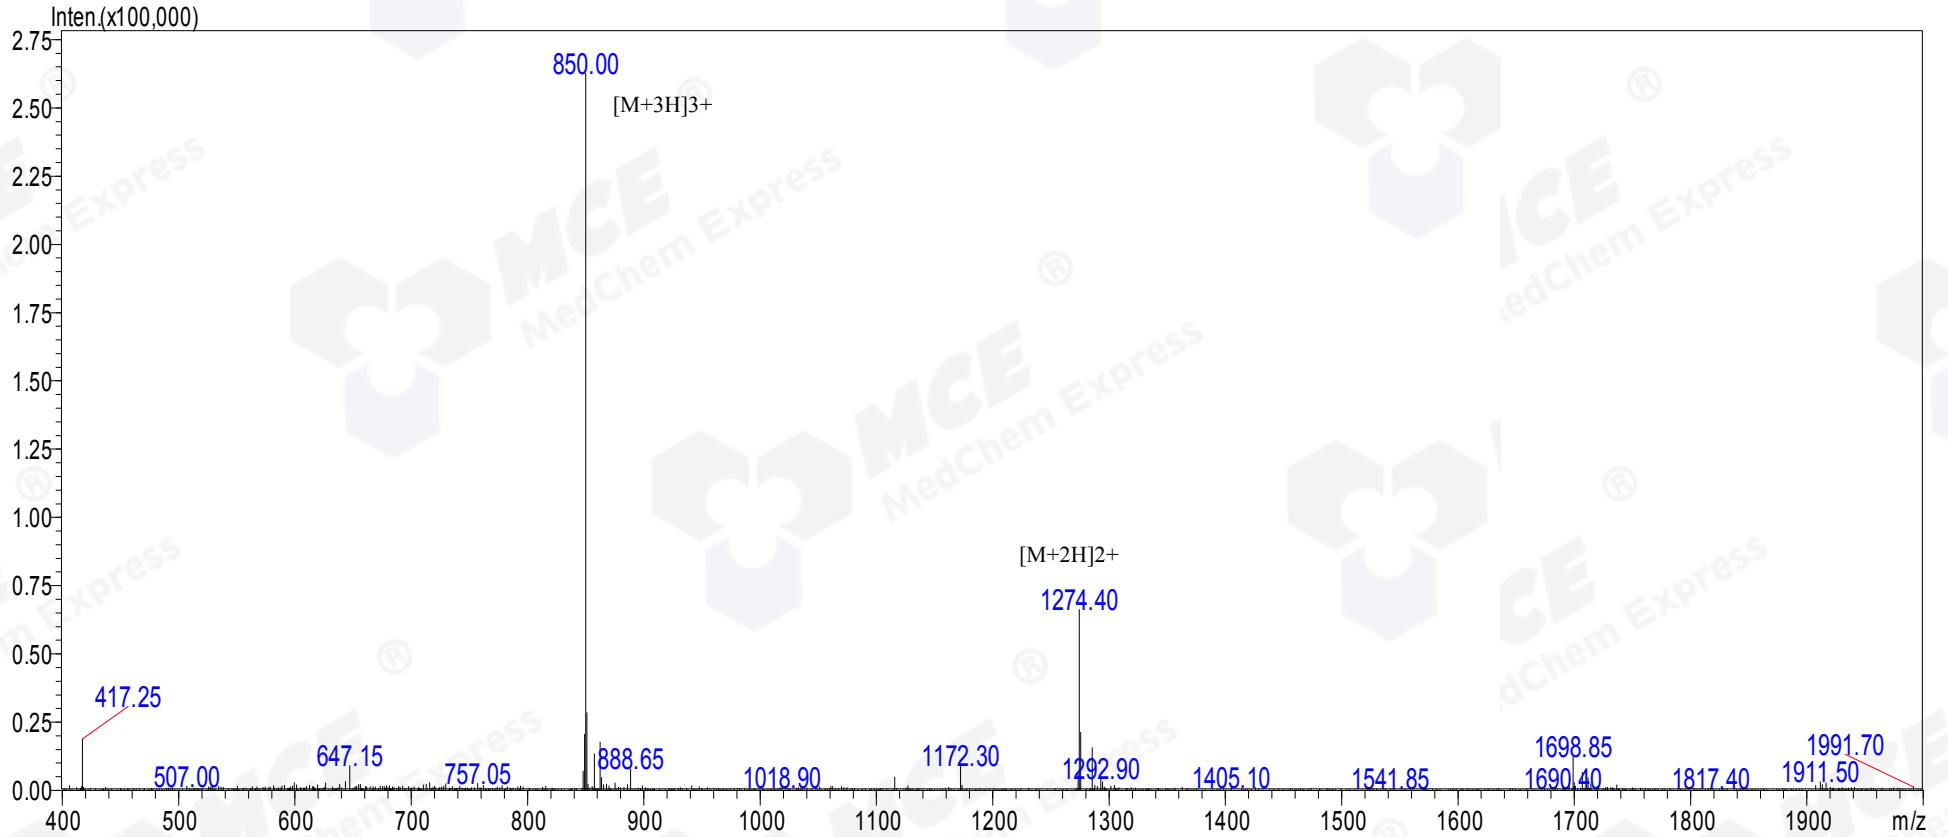

Sample Description

Analyzed date: 2020-11-20  
 Analyst: SHAO  
 Sample: 601479  
 M.W.: 2547.0  
 Lot. No.:

Instrument

Probe: ESI  
 Nebulizer Gas Flow: 1.5L/min  
 CDL: -20.0v  
 CDL Temp.: 250°C  
 Block Temp.: 200°C

SHIMADZU LCMS-2020

Probe Bias: +4.5kv  
 Detector: 1.5kv  
 T. Flow: 0.2ml/min  
 B. Conc.: 50%H2O/50%ACN