


Data file: C:\CHEM32\1\DATA\201120\601479_20100051Final.D
 Catalog No: HY-P0207A
 Description: Mobile phase: Buffer A: 0.1%TFA in H2O
 Buffer B: 0.1%TFA in ACN
 Gradient: 31-41% in 20min, Flow rate: 1.0ml/min
 Column: Uni tary C18, 4. 6*150mm, 5um 100A (A-007)
 Instrument: Agilent HPLC 1100

Instrument: 1100
 Injection date: 2020/11/20 10: 38: 50
 Last changed: 2020/11/20 11: 12: 21

Location: 22
 Injection: 1 of 1
 Injection volume: 10.000
 Acq. operator: QC

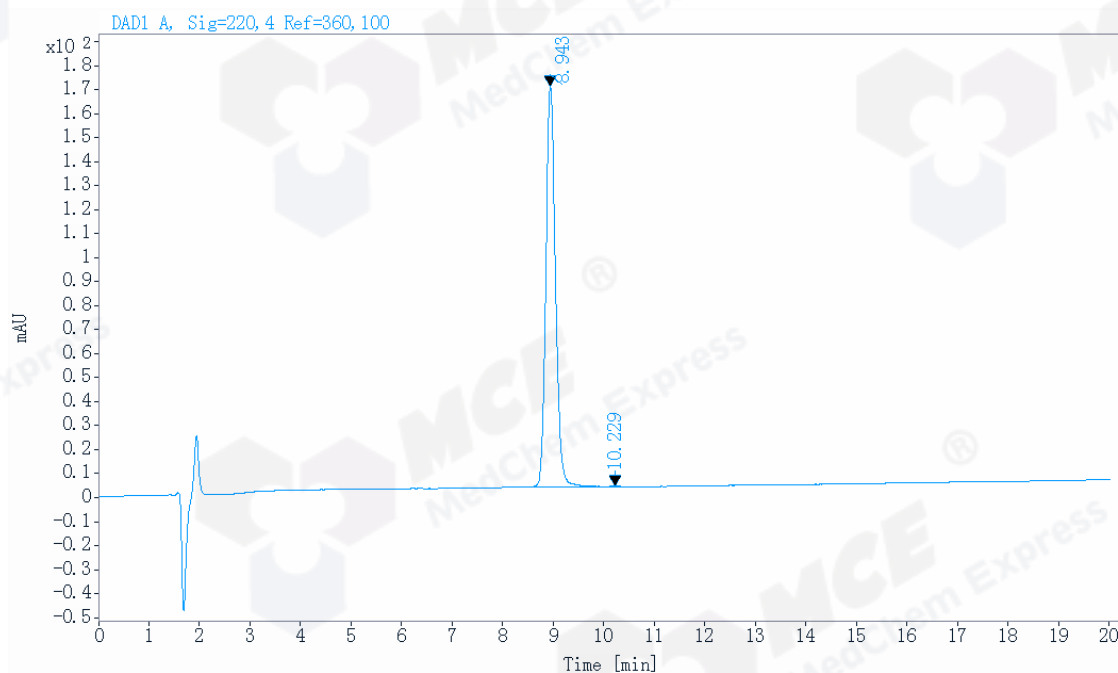

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[mi n]	Type	Width[mi n]	Area	Height	Area% Name
8.943	MF	0.2205	2214.9221	167.4333	99.8291
10.229	FM	0.1913	3.7914	0.3304	0.1709
Sum			2218.7135		