


MS Spectrum

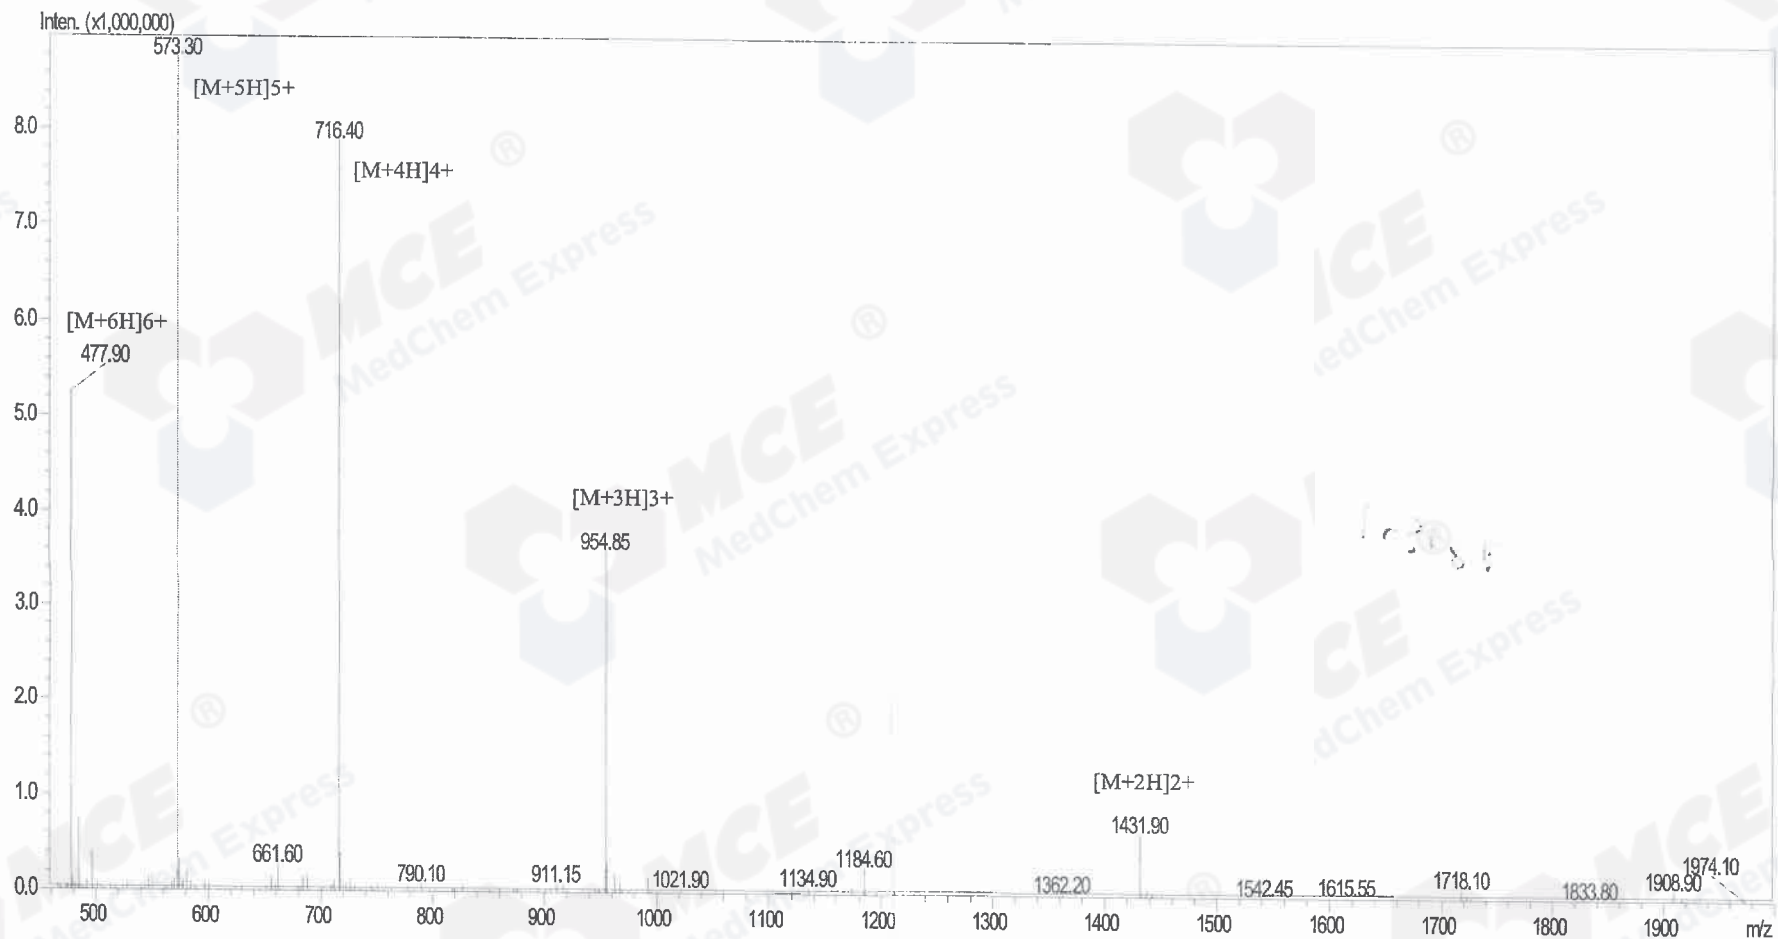

Data and Time : 2019/4/16  
Sample : 3\*flag peptide MK-23  
Inj. Volume : 1.000  
Mw : 2861.93  
Catalog No : HY-P0319A Batch# 40389

Probe : ESI  
Nebulizer Gas Flow : 1.5L/min  
CDL : -20.0v  
CDL Temp : 250°C  
Block Temp : 400°C  
Probe bias : -4.5kv  
Detector : 1.2kv  
T.Flow : 0.2ml/min  
B.conc : 50%H2O/50%ACN