


# MASS SPECTROMETRY REPORT

P171012-5-Y2-1107 17 (0.314) Cm (14:20)

Scan ES+  
5.86e6

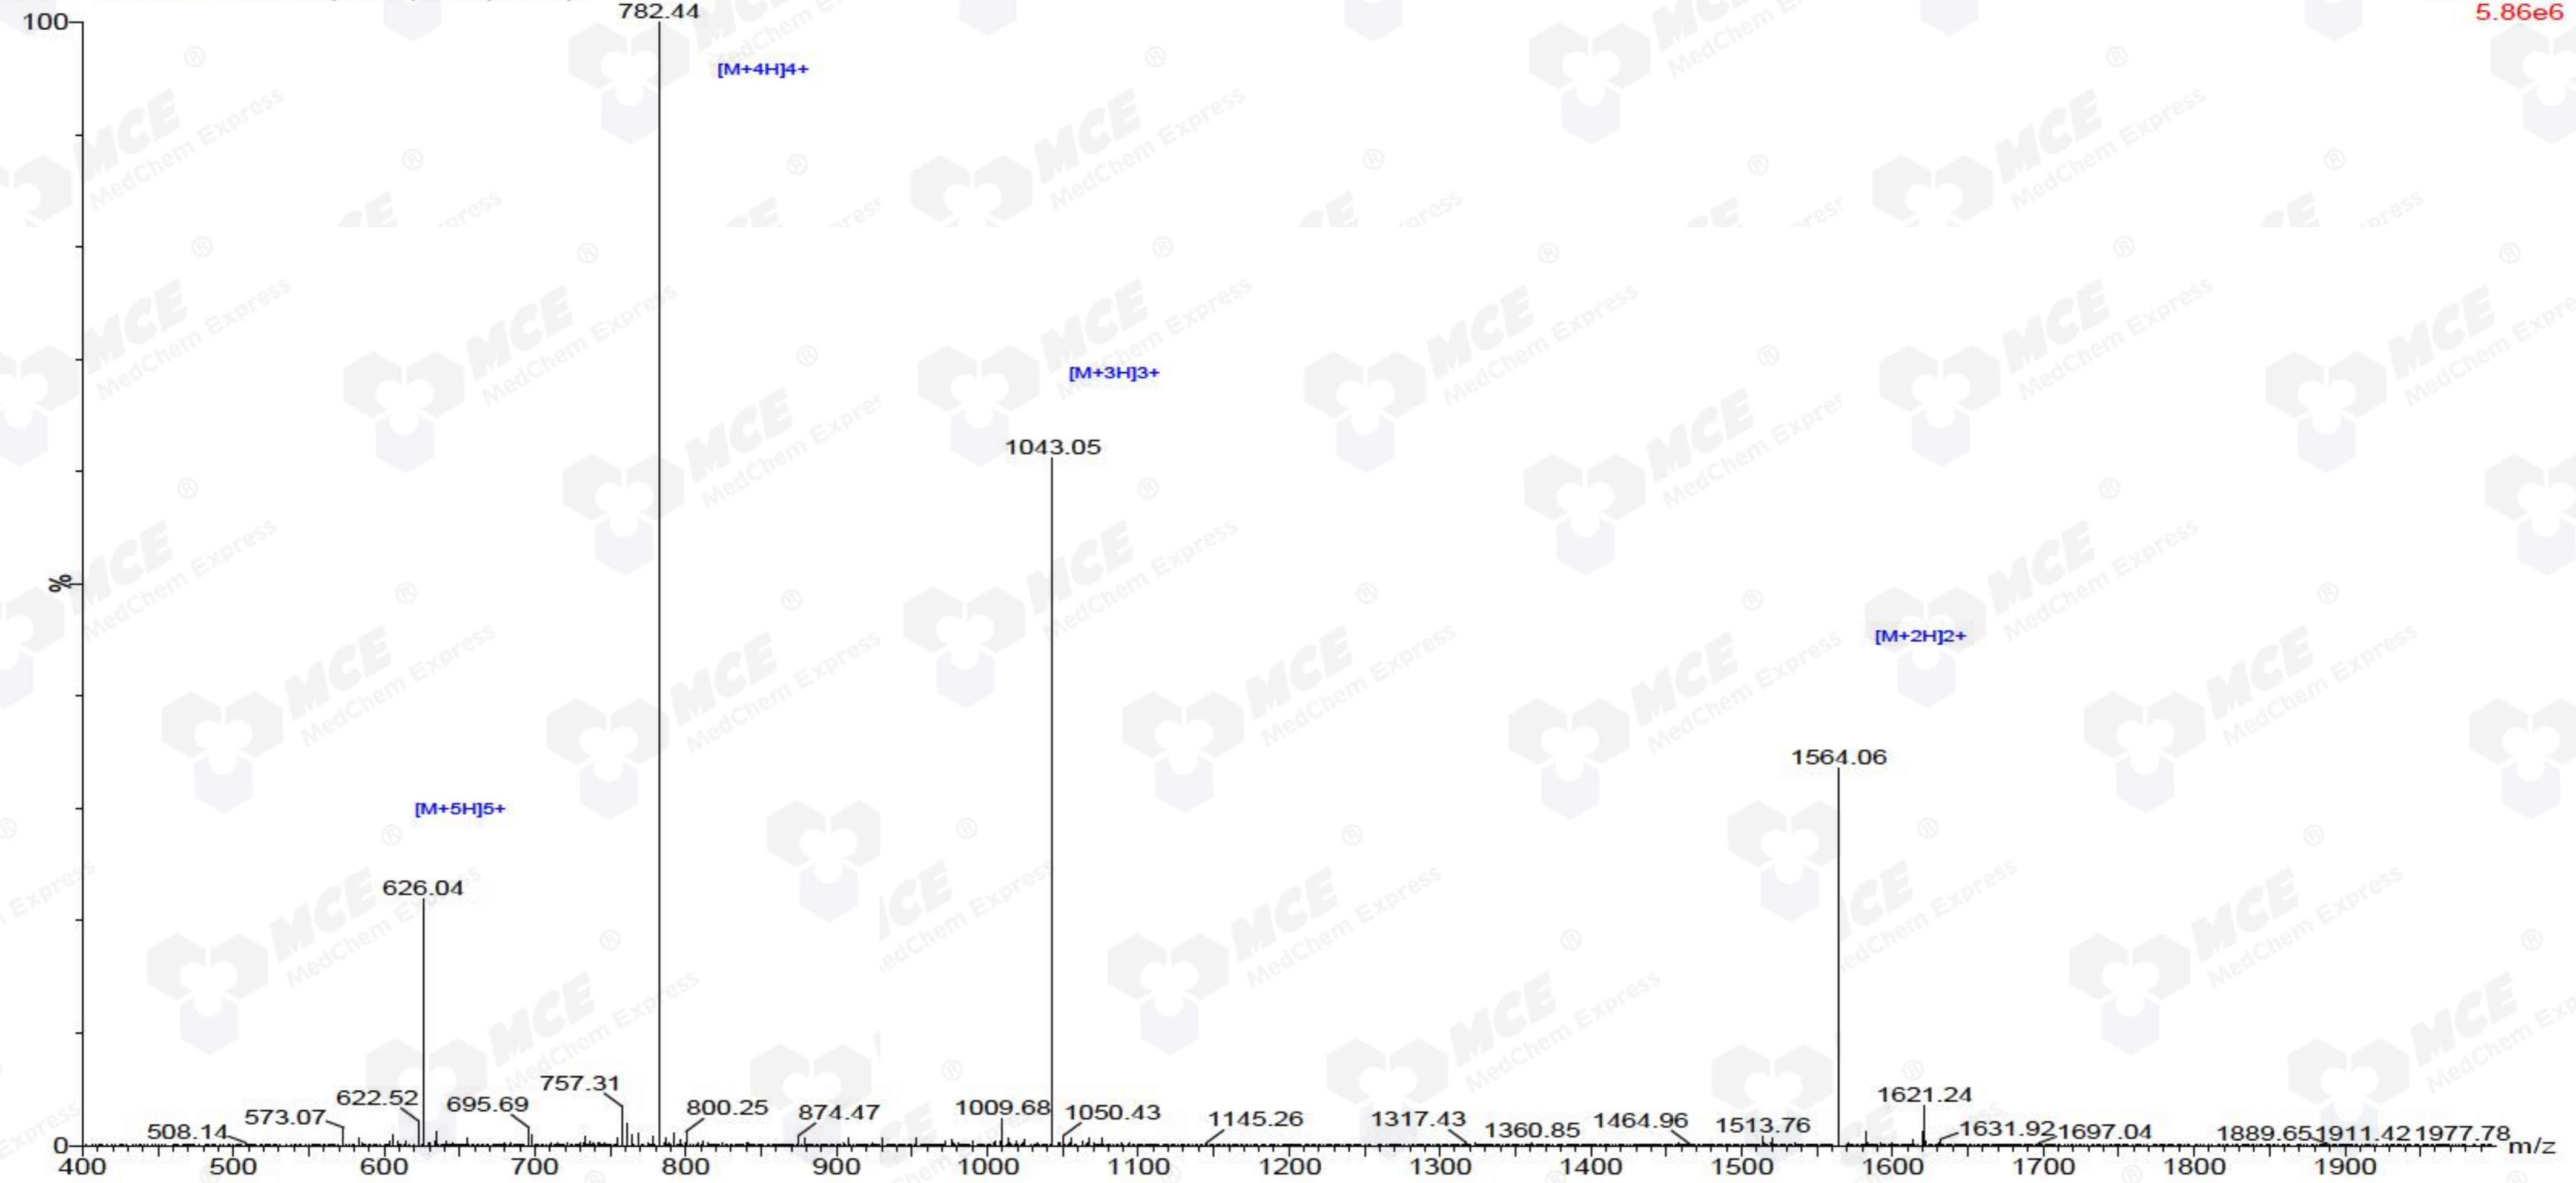

## Sample Description

Analyzed date: 2017-11-14  
Analyst: PY  
Sample: HCGRP-(8-37) CAS: 119911-68-1  
M.W.: 3125.65  
Catalog No: HY-P1014 Batch#27346

## Instrument

Waters ZQ2000  
Probe: ESI  
Nebulizer Gas Flow: 1.5L/min  
CDL: -20.0v  
CDL Temp.: 250 °C  
Block Temp.: 200 °C

## Waters ZQ2000

Probe Bias: +4.5kv  
Detector: 1.5kv  
T. Flow: 0.2ml/min  
B. Conc.: 50%H2O/50%ACN