

File ..1\DATA\2019\20190505\558\BIZ2019-430-WYQ1.D Tgt Mass (CHM):

Injection Date : 5 May 19 10:59 am +0800 Seq. Line : 14

Sample Name : BIZ2019-430-WYQ1 Location : P2-E-09

Acq. Operator : LQ_1052 Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\Chem32\1\data\2019\20190505\558\1-POS-3MIN-1.M

Analysis Method : D:\CHEM32\1\DATA\2019\20190505\558\1-POS-3MIN-1.M

Catalog No : HY-P1276A Batch#40703





Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)

Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min

Column :SunFire C18, 4.6*50mm,3.5um A-RP-322

Oven Temperature : 45

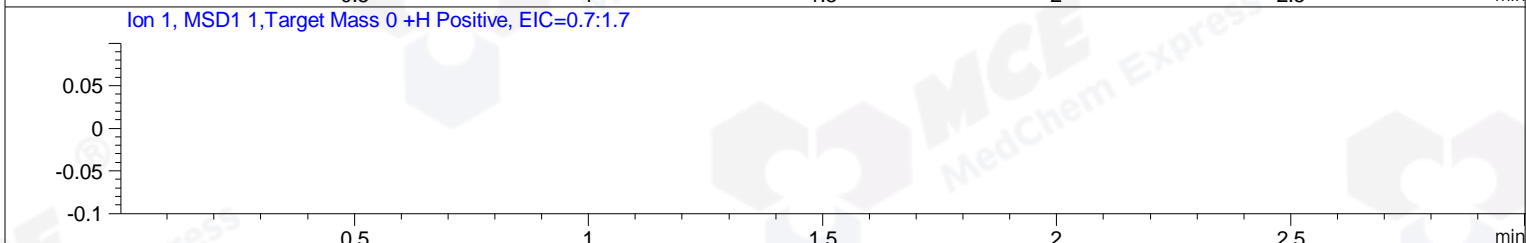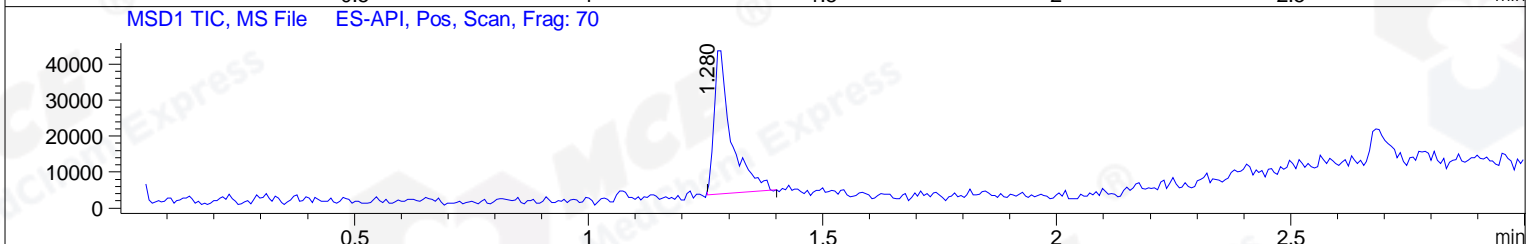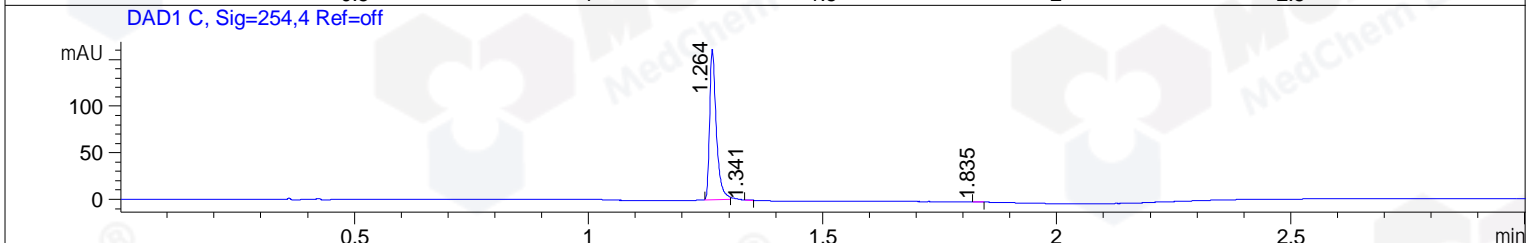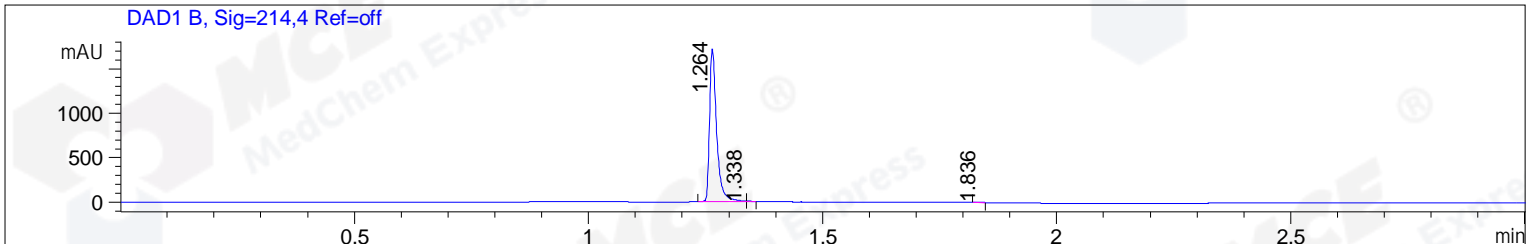

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.26	0.02	1819.98	1720.71	99.76	541
1.34	0.01	3.55	5.49	0.19	541
1.84	0.01	0.74	0.83	0.04	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.26	0.01	161.31	162.01	99.68	541
1.34	0.01	0.31	0.48	0.19	541
1.83	0.01	0.22	0.25	0.13	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.28	0.03	102288.98	41504.64	100.00	541

Ret. Time: 1.28

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

