



Ret. Time: 0.39

<<<< POSITIVE SPECTRA >>>>

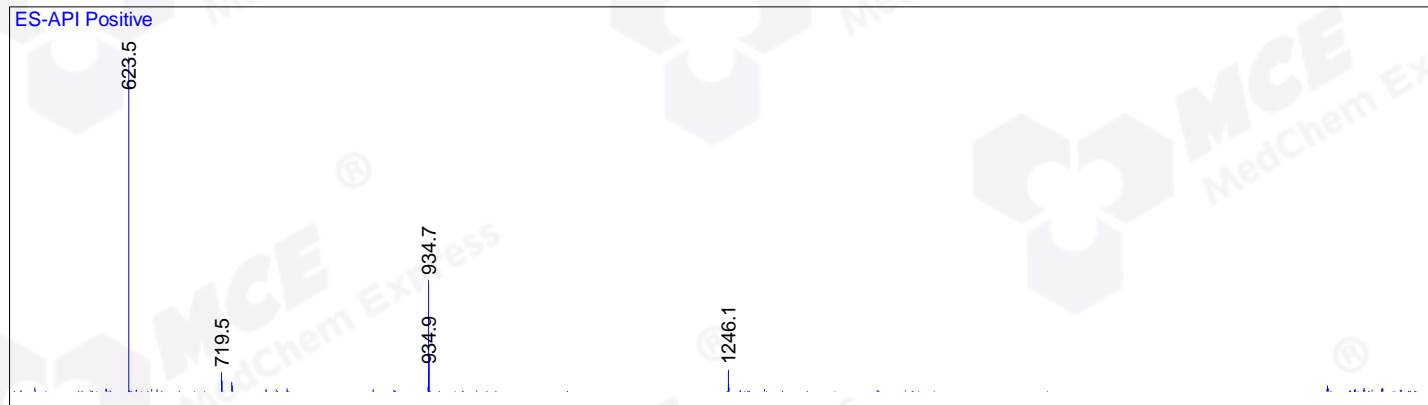


Ret. Time: 1.07

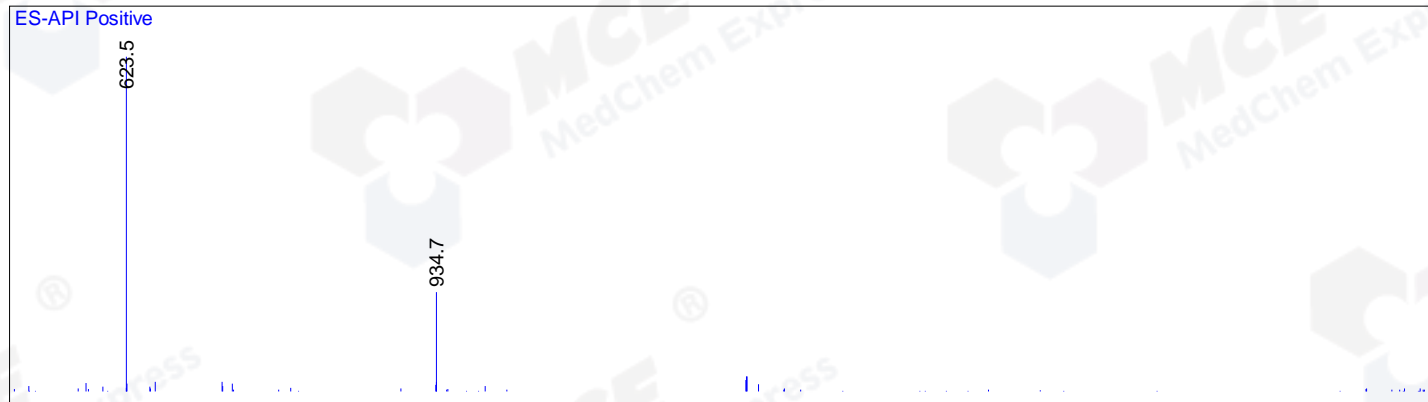

MS Spectrum

Positive

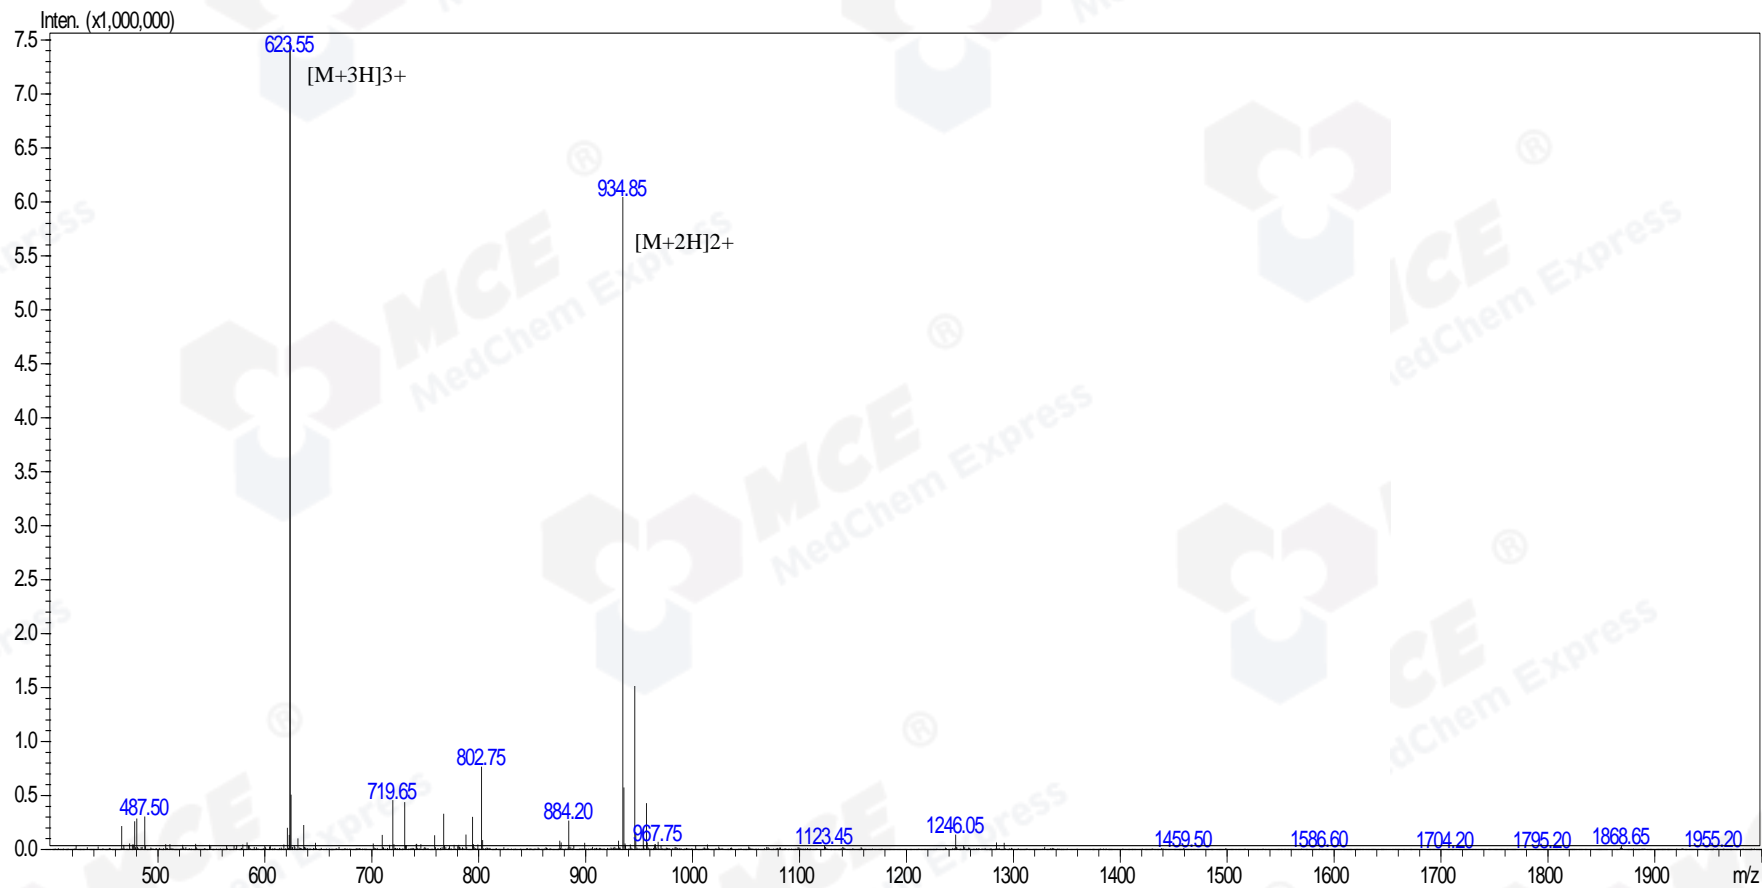

Acquired by :Shen
Data Acquired : 2020/12/17
Injection Volume : 1
Sample Name : TI-17-NH2
Mw : 1868.06
Product Name : PKA Inhibitor Fragment (6-22) amide (TFA)

Probe :ESI
Nebulizer Gas Flow :1.5L/min
CDL :-20.0v
CDL Temp :250°C
Block Temp :400°C
Probe bias :+4.5kv
Detector :1.2kv
T.Flow :0.2ml/min
B.conc :50%H2O/50%ACN